

FIG. 1

FIG. 3

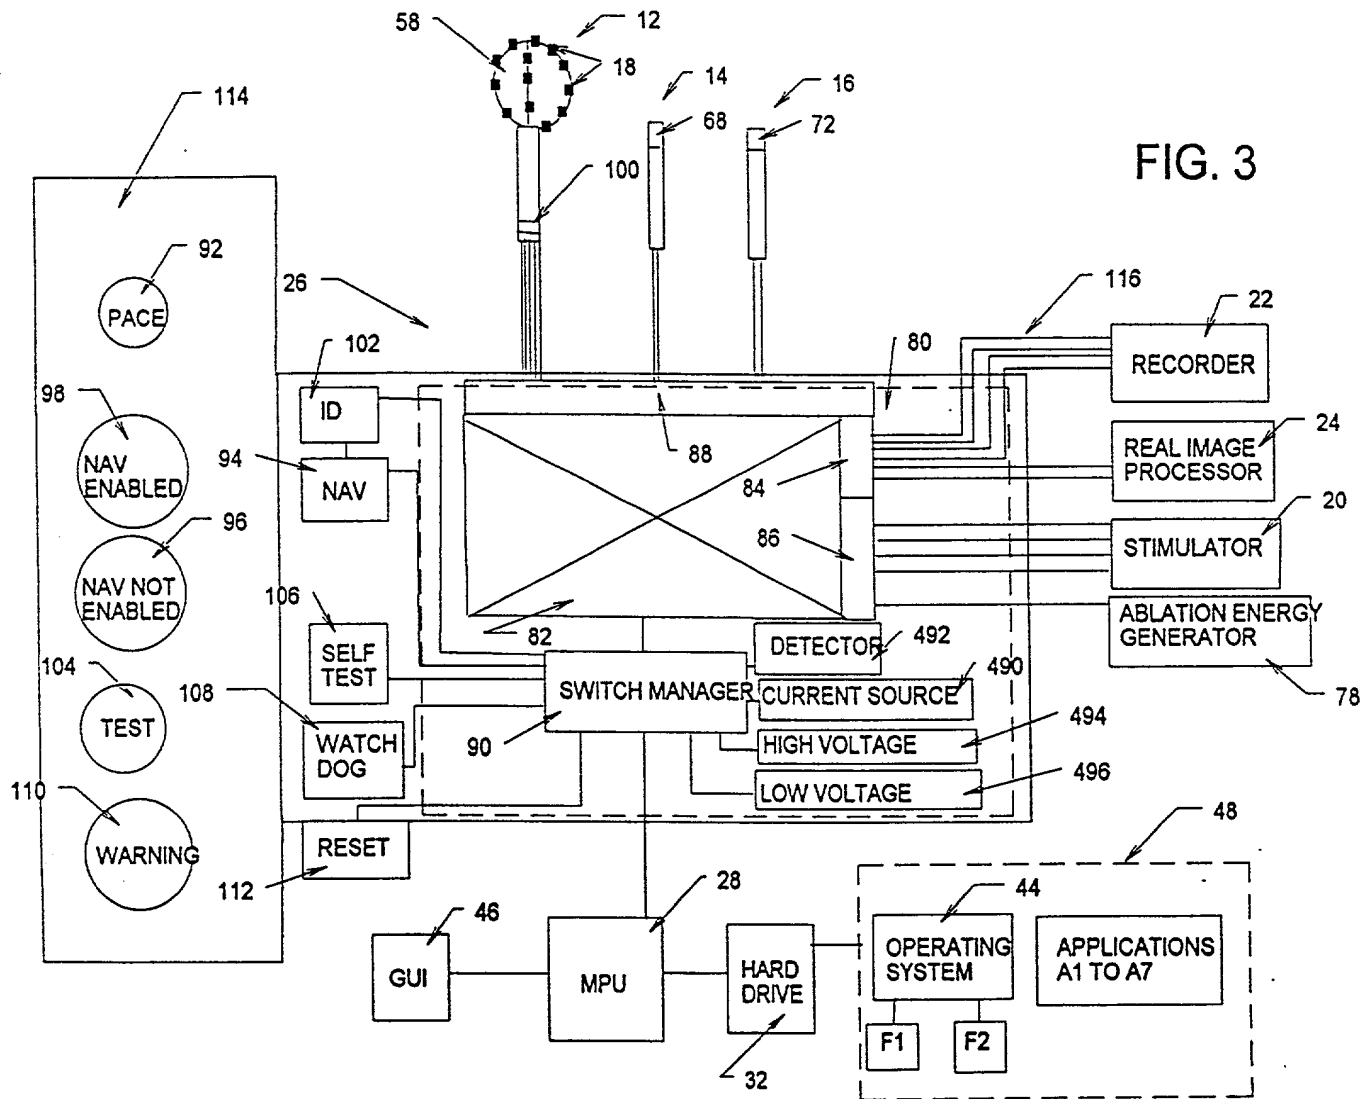


FIG. 4 is a schematic diagram of a start up screen of a medical device. The screen displays a logo and a menu of options. The options are: Recording Protocols, Pacing Protocols, Virtual Image Navigation, Real Image Navigation, Test, Print, Service, and Event Log OFF.

Start Up Screen
Logo

FIG. 4

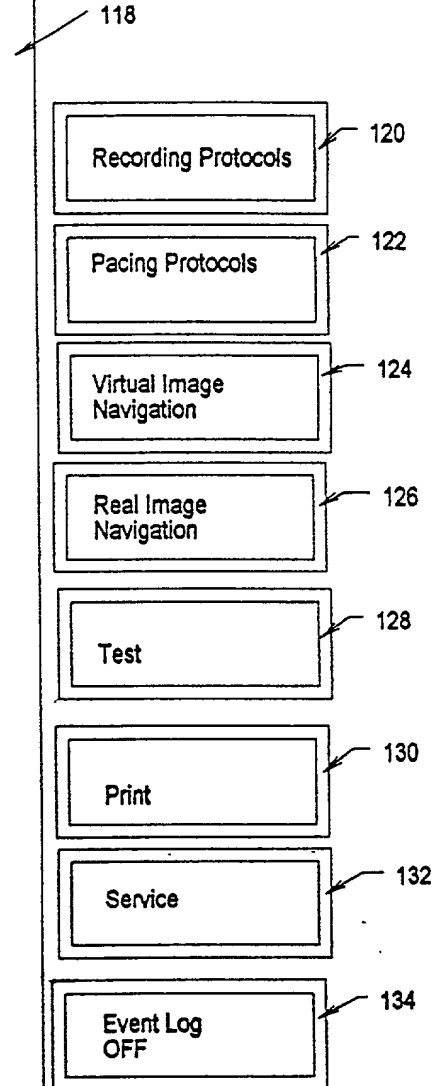


FIG. 5

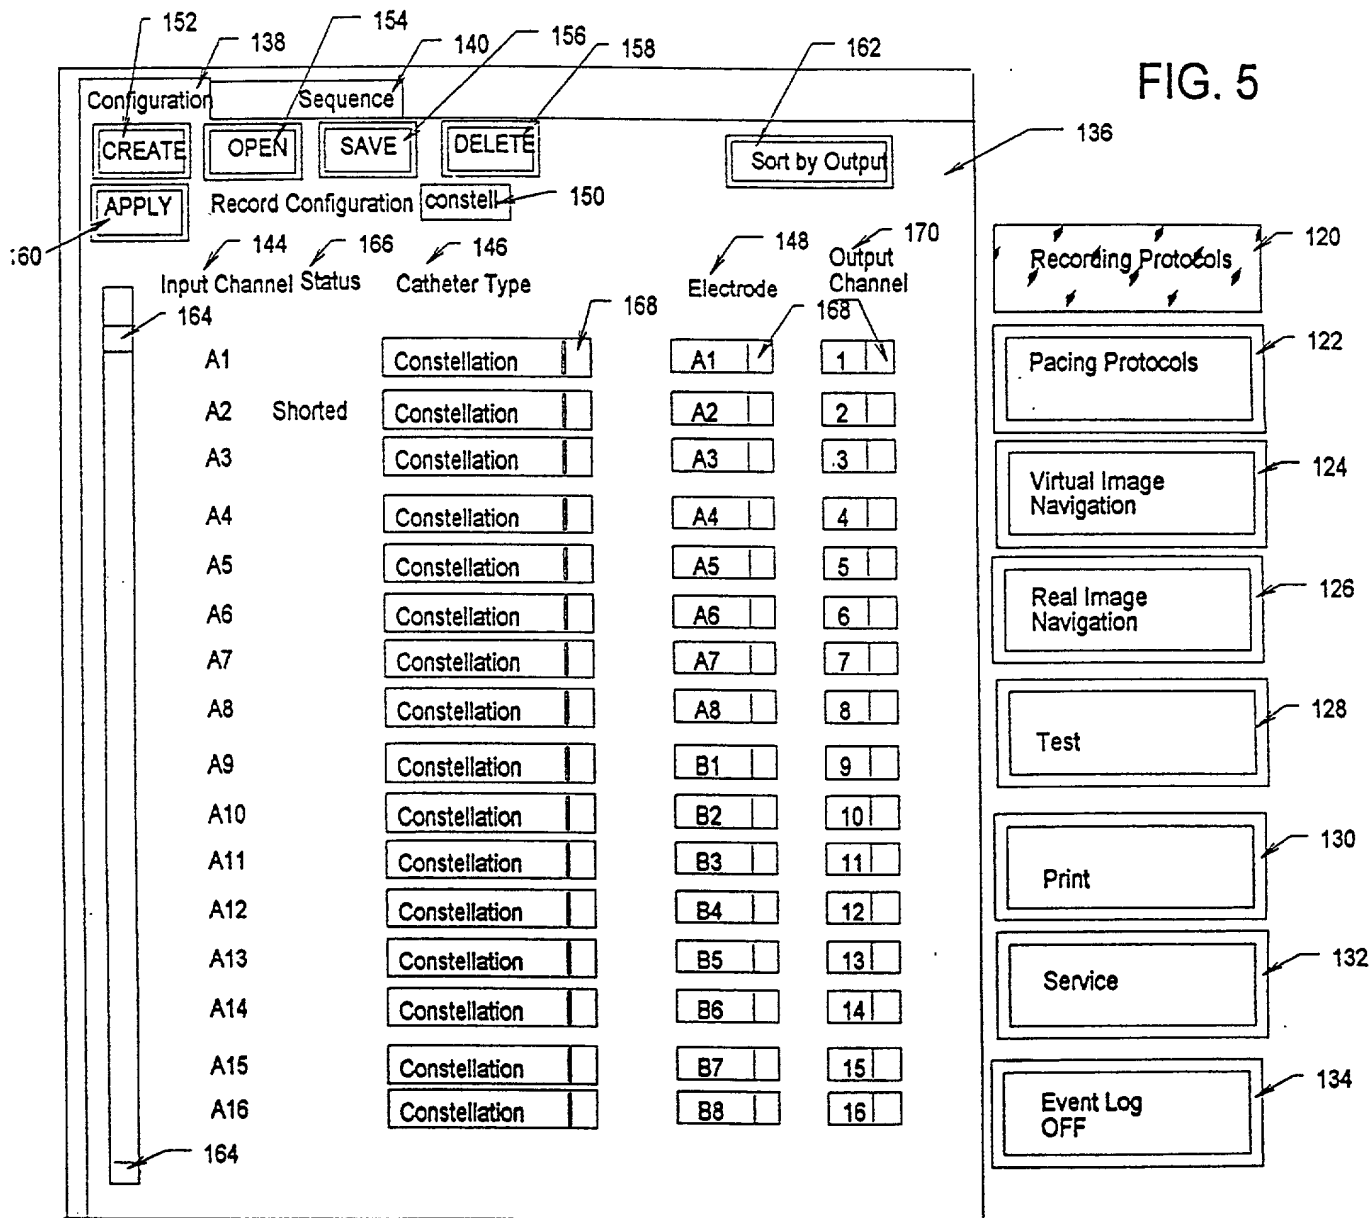
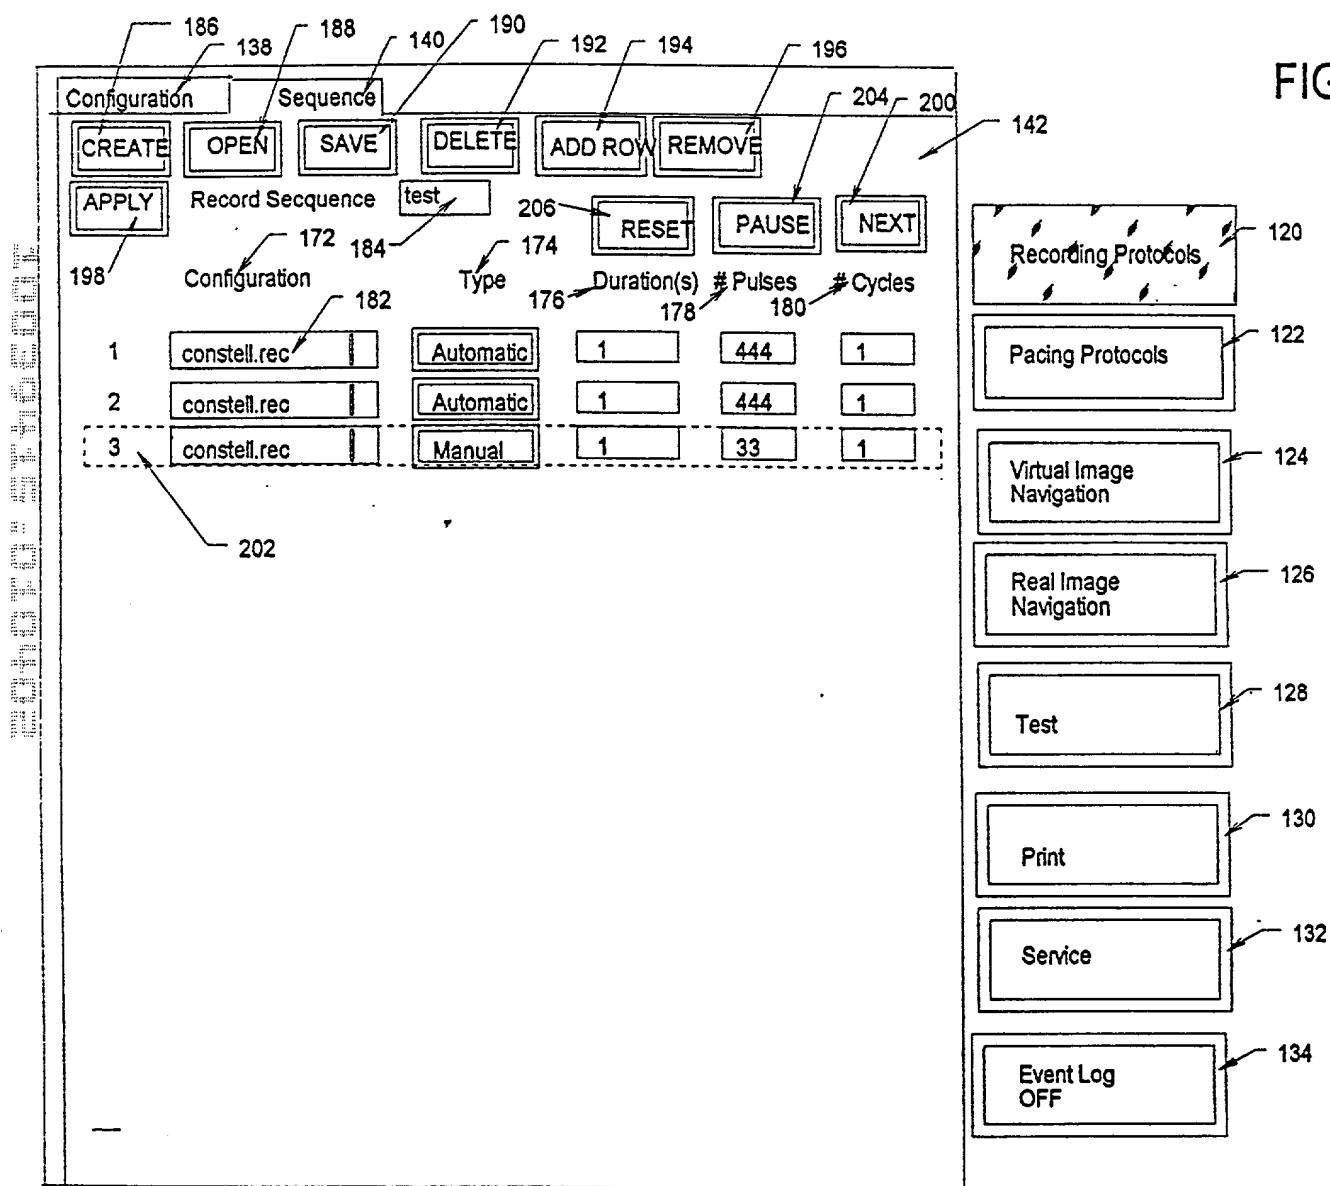


FIG. 6



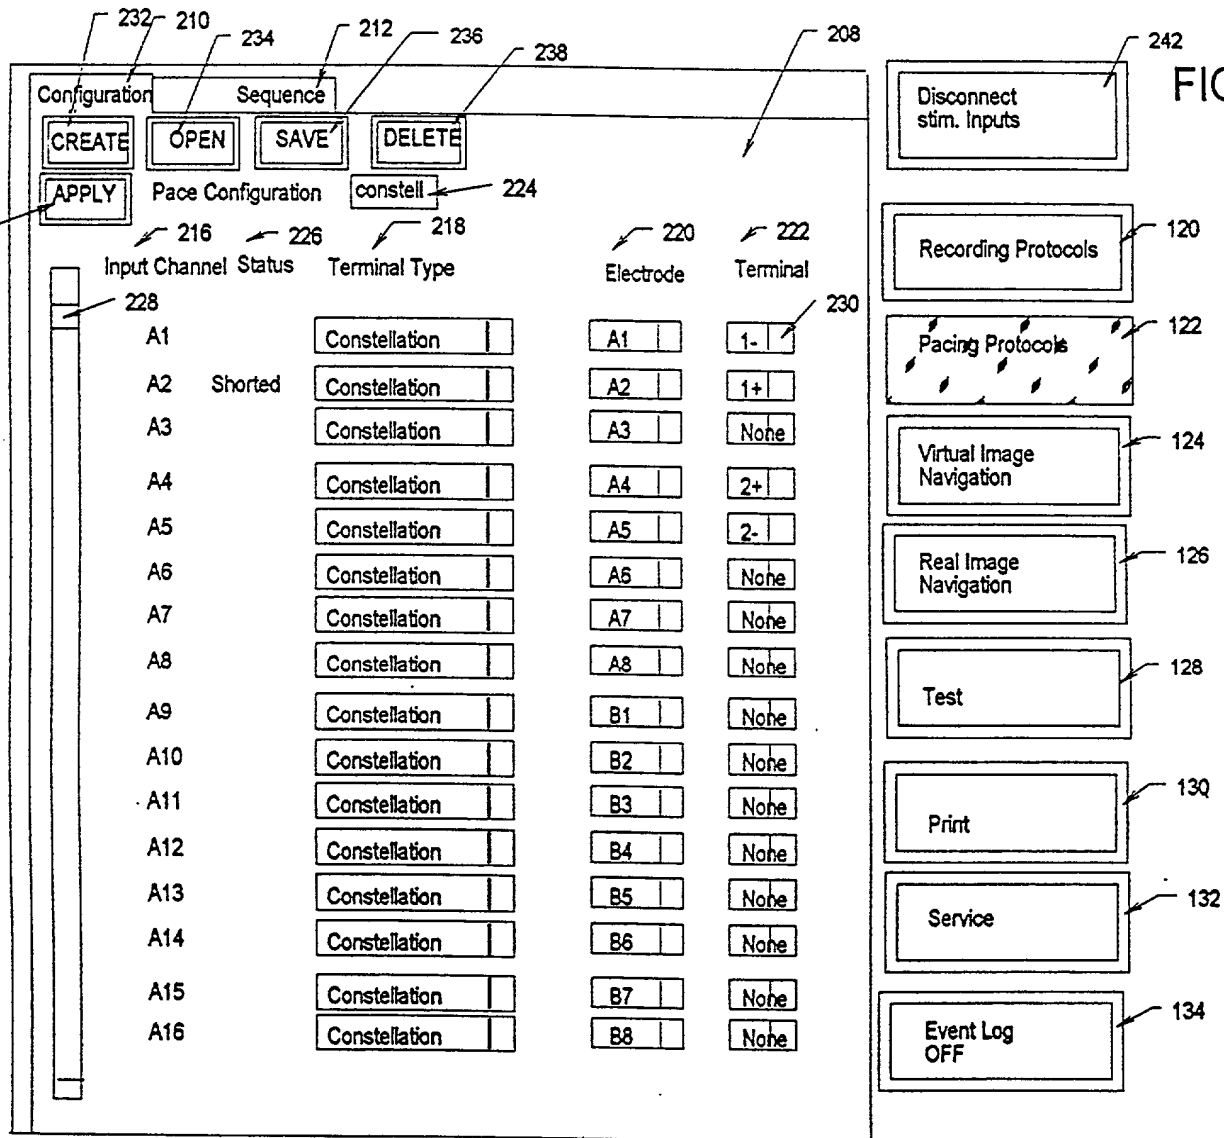
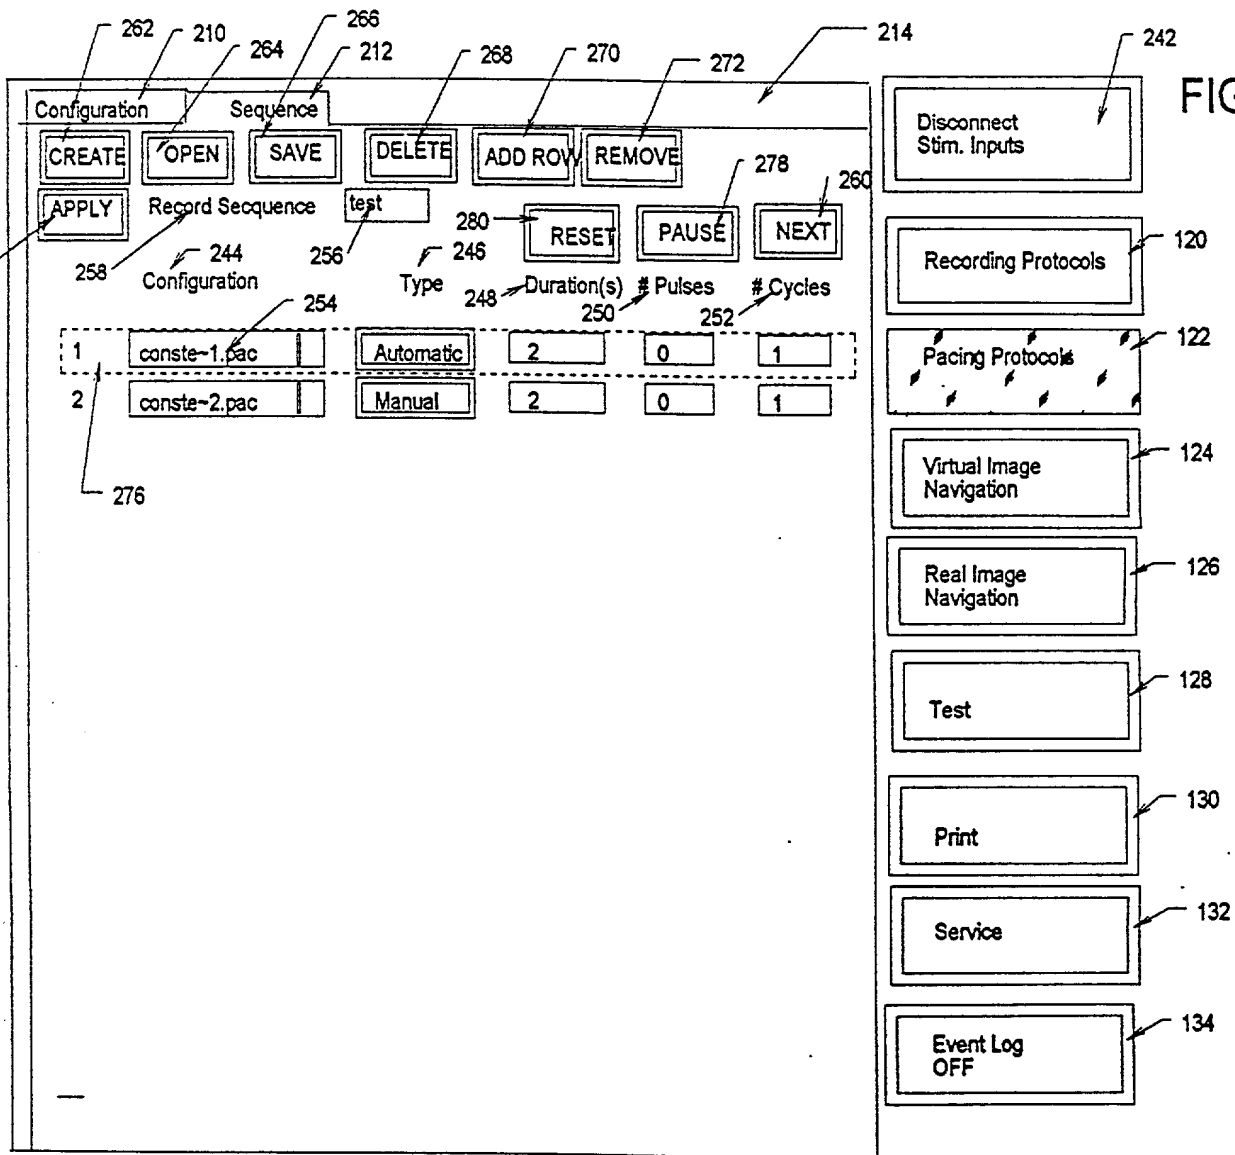


FIG. 8 is a block diagram of a user interface for a medical device, showing a main menu and a sub-menu.



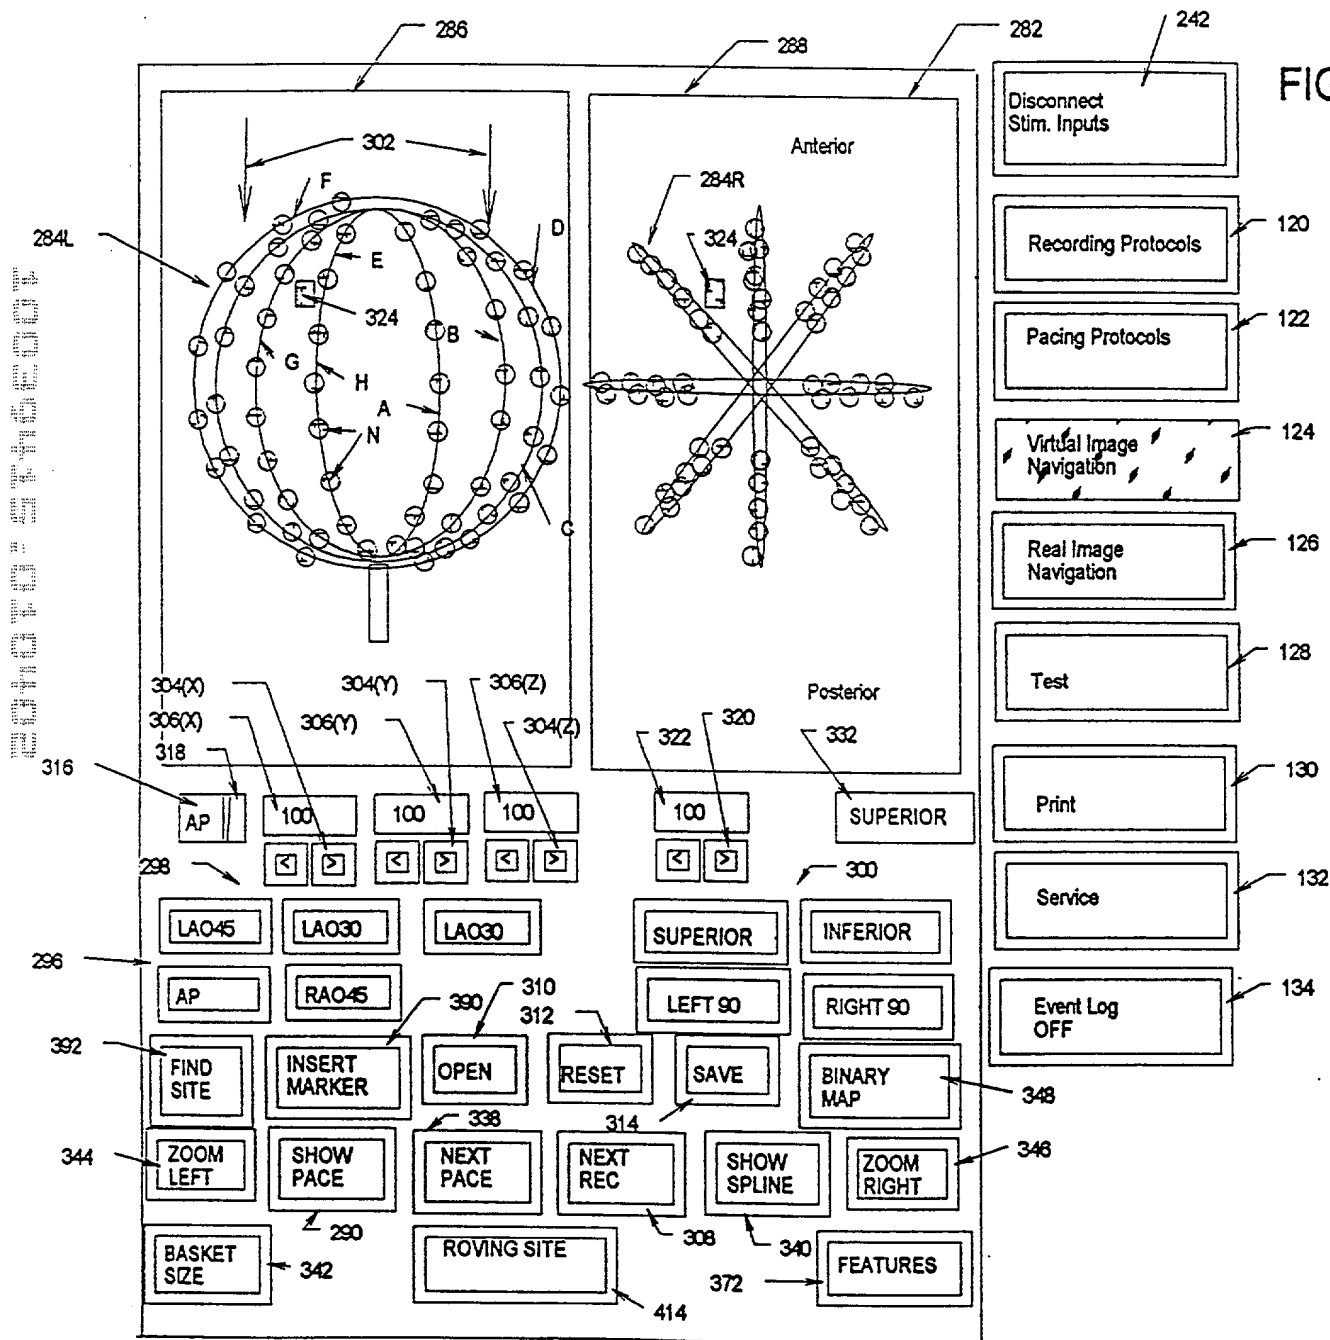


FIG. 9

FIG. 10

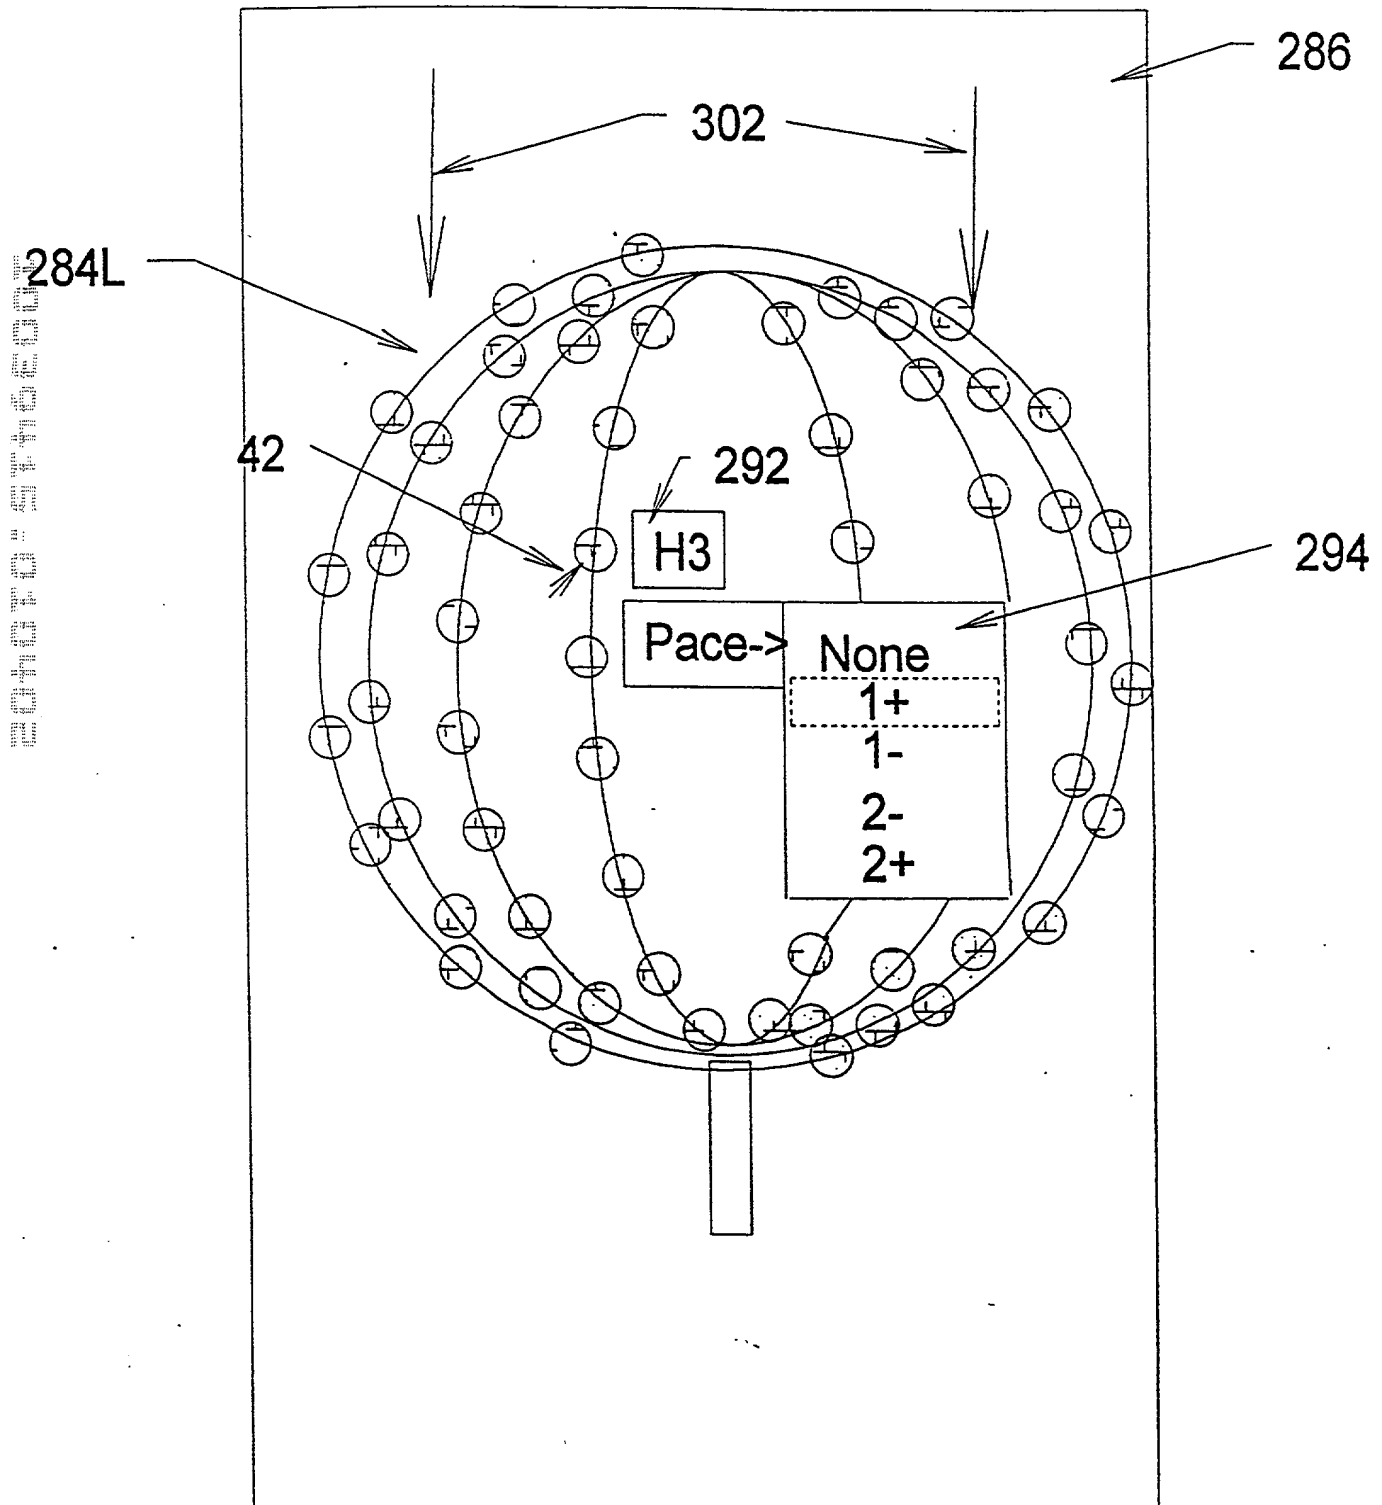


FIG. 11

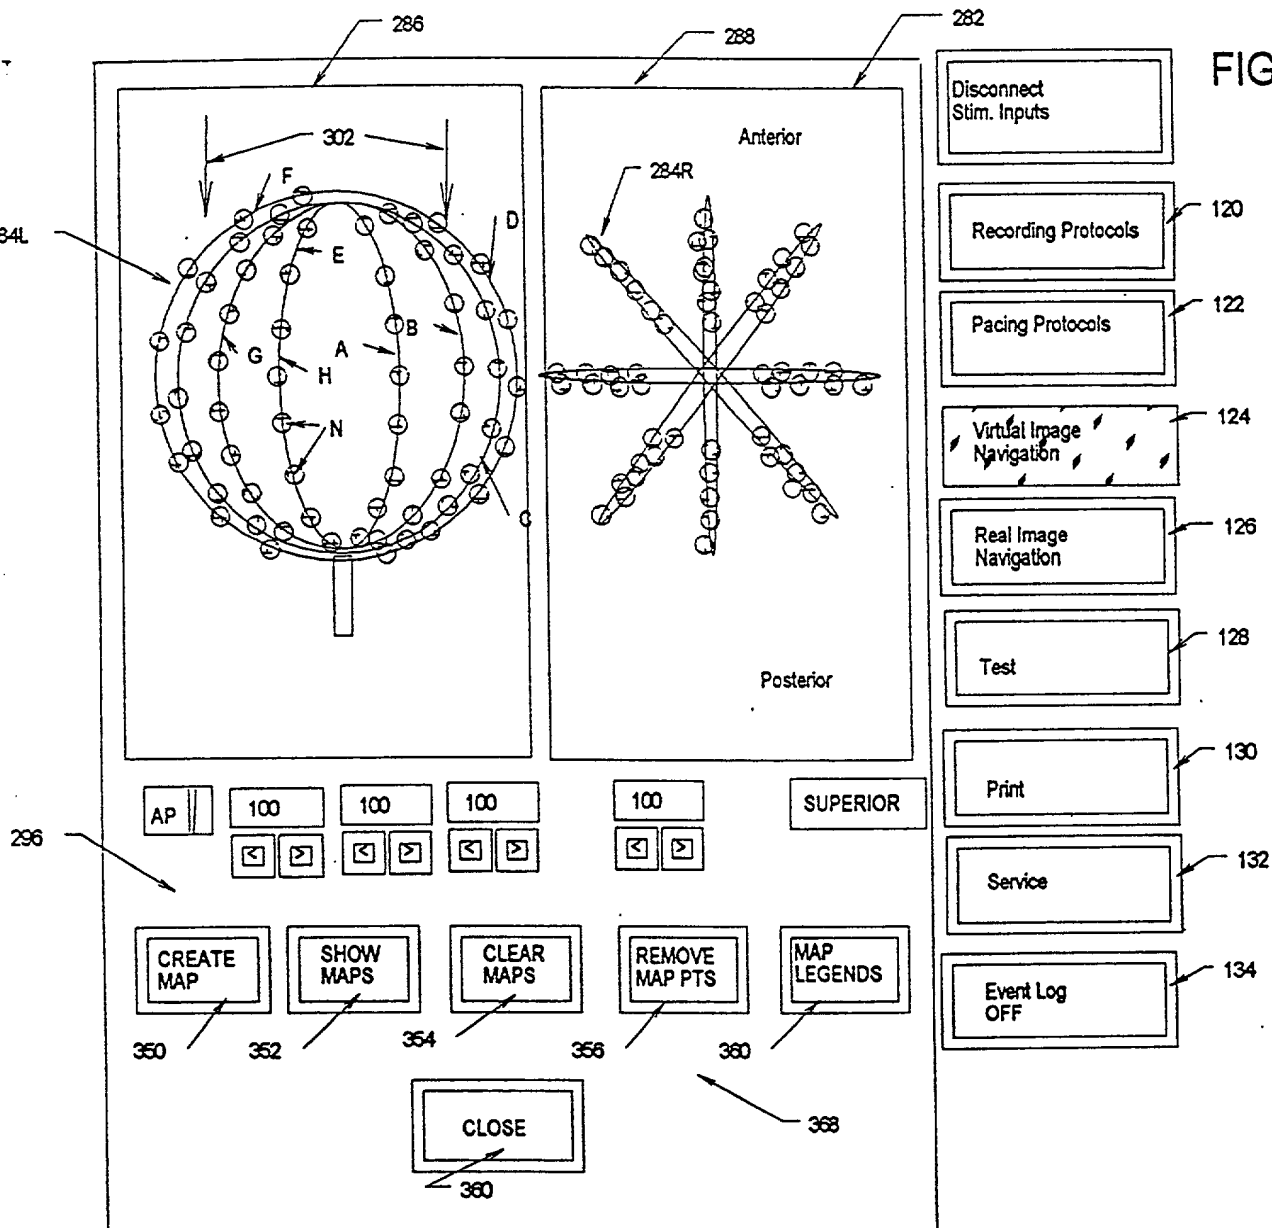


FIG. 12

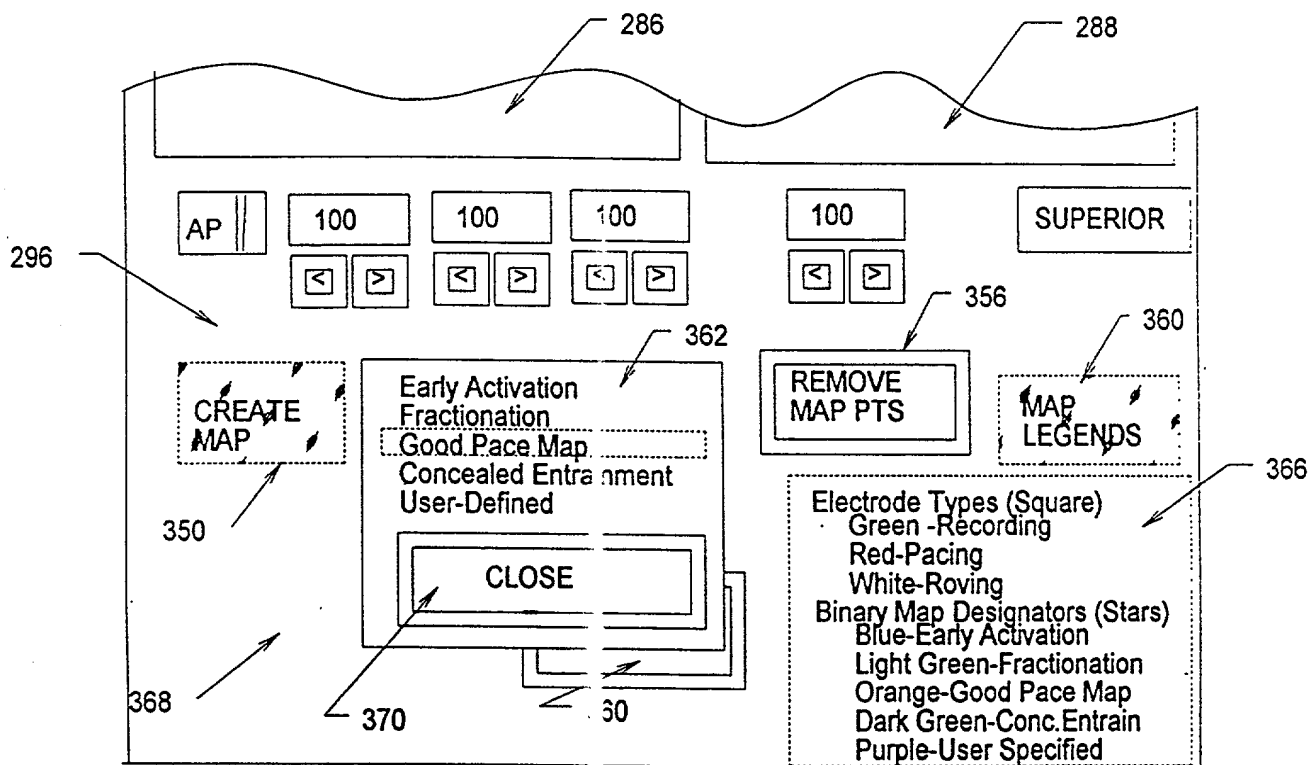
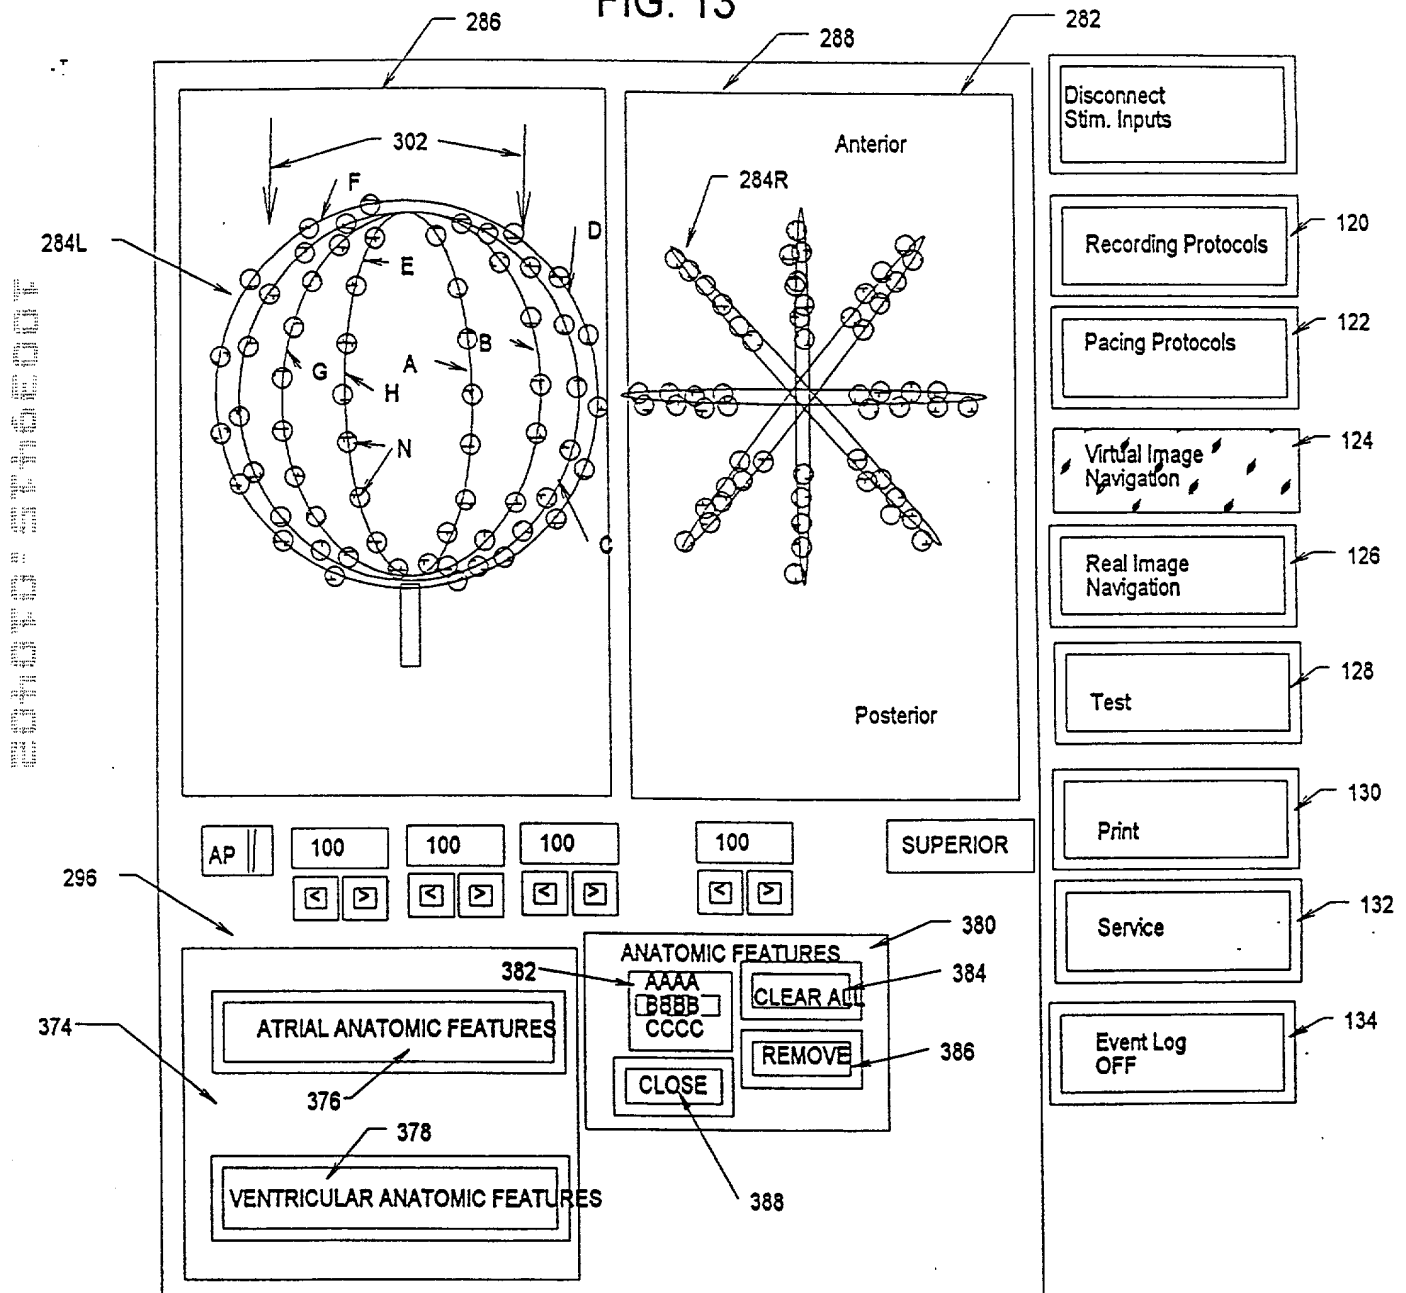


FIG. 13



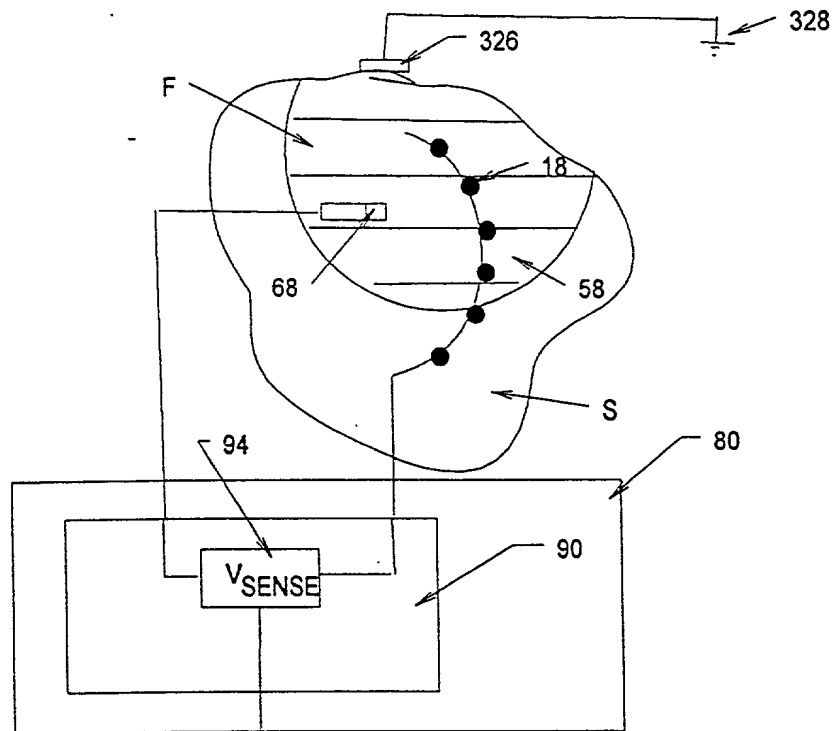


FIG. 14

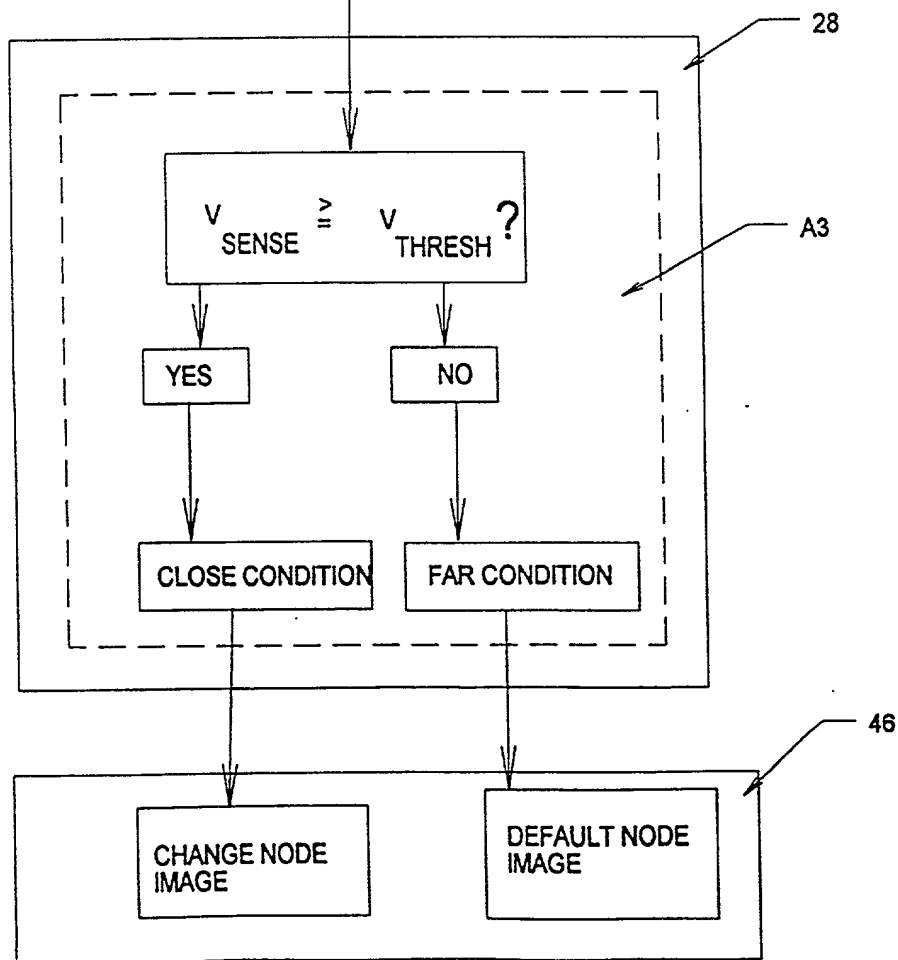


FIG. 15

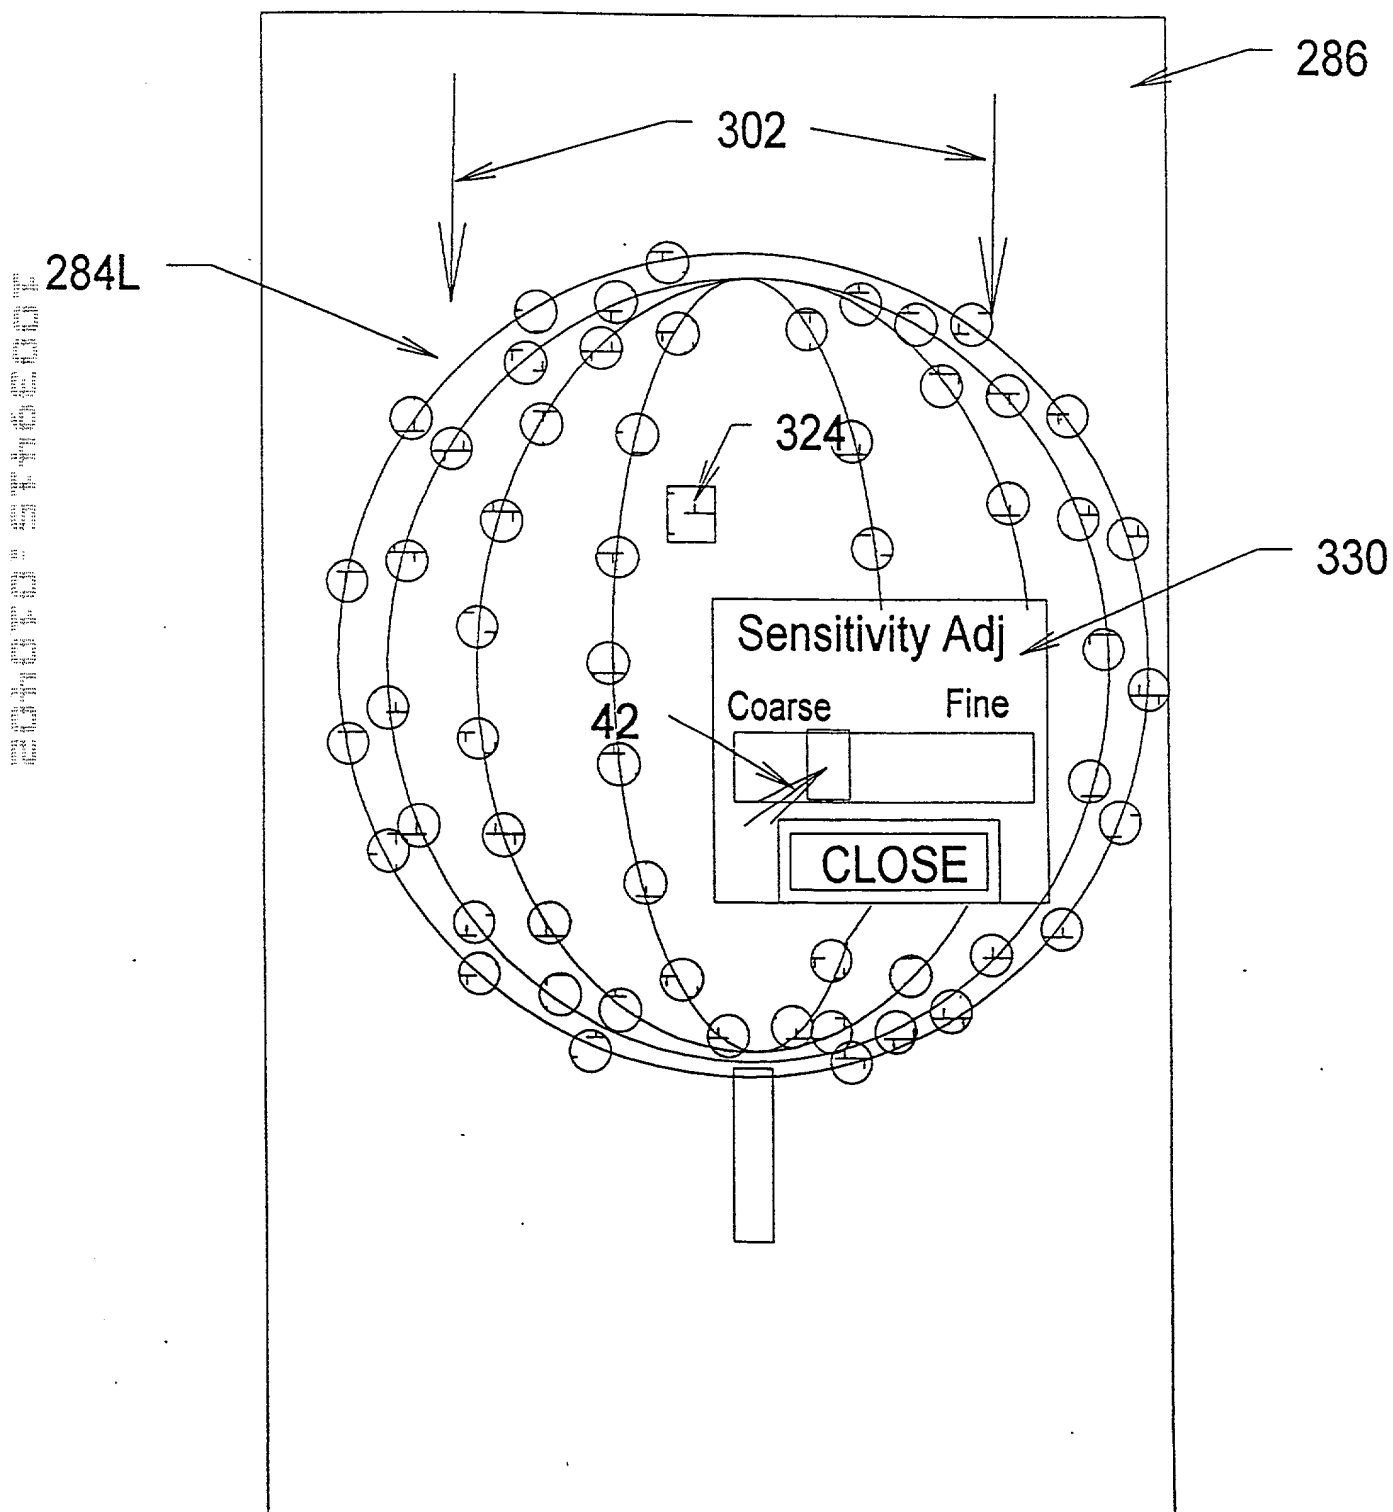


FIG. 16

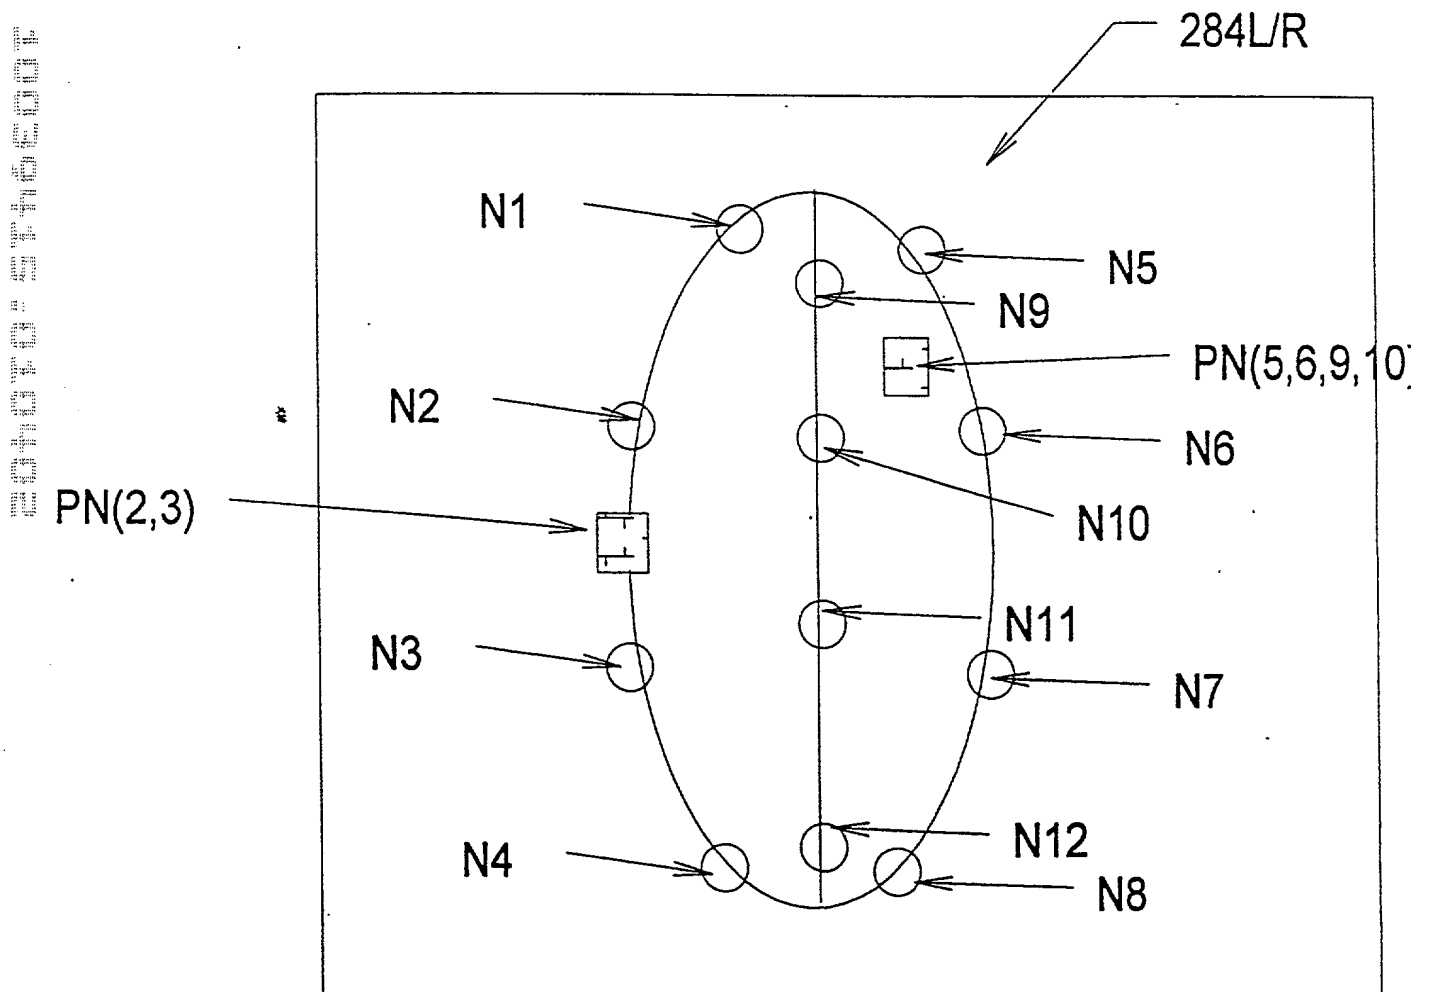


FIG. 17

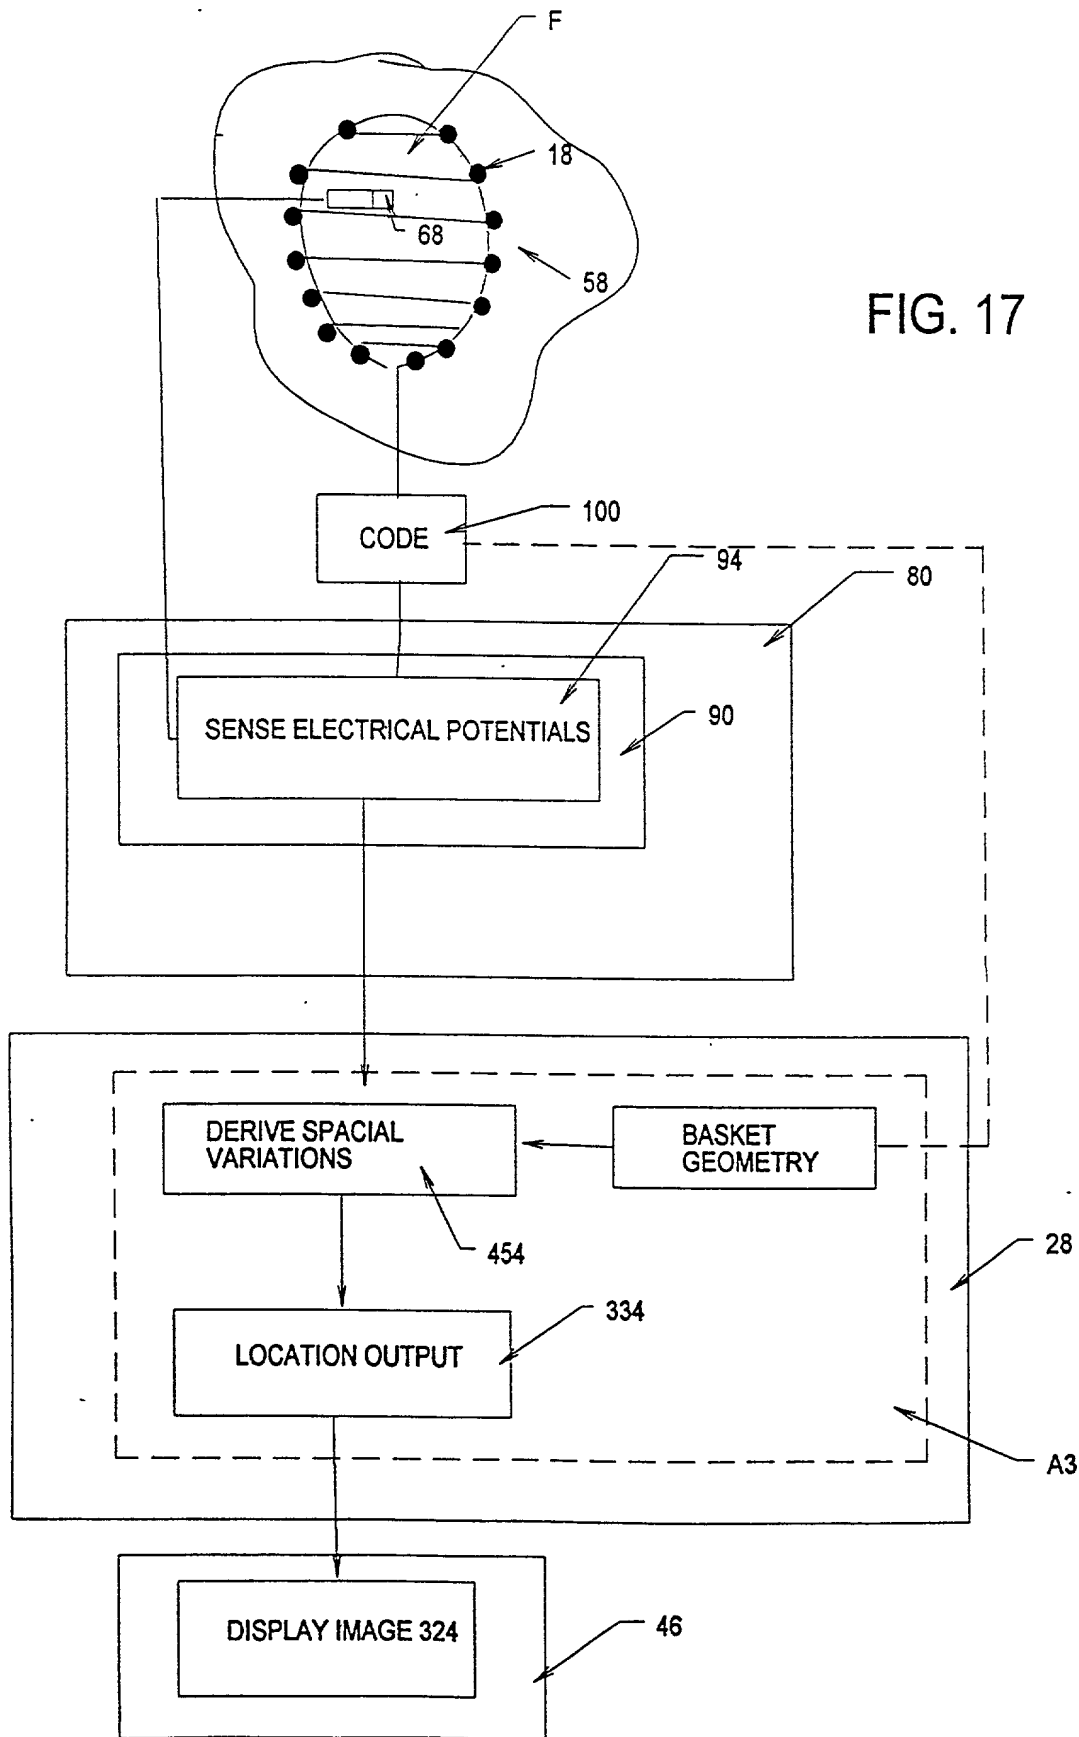


FIG. 18

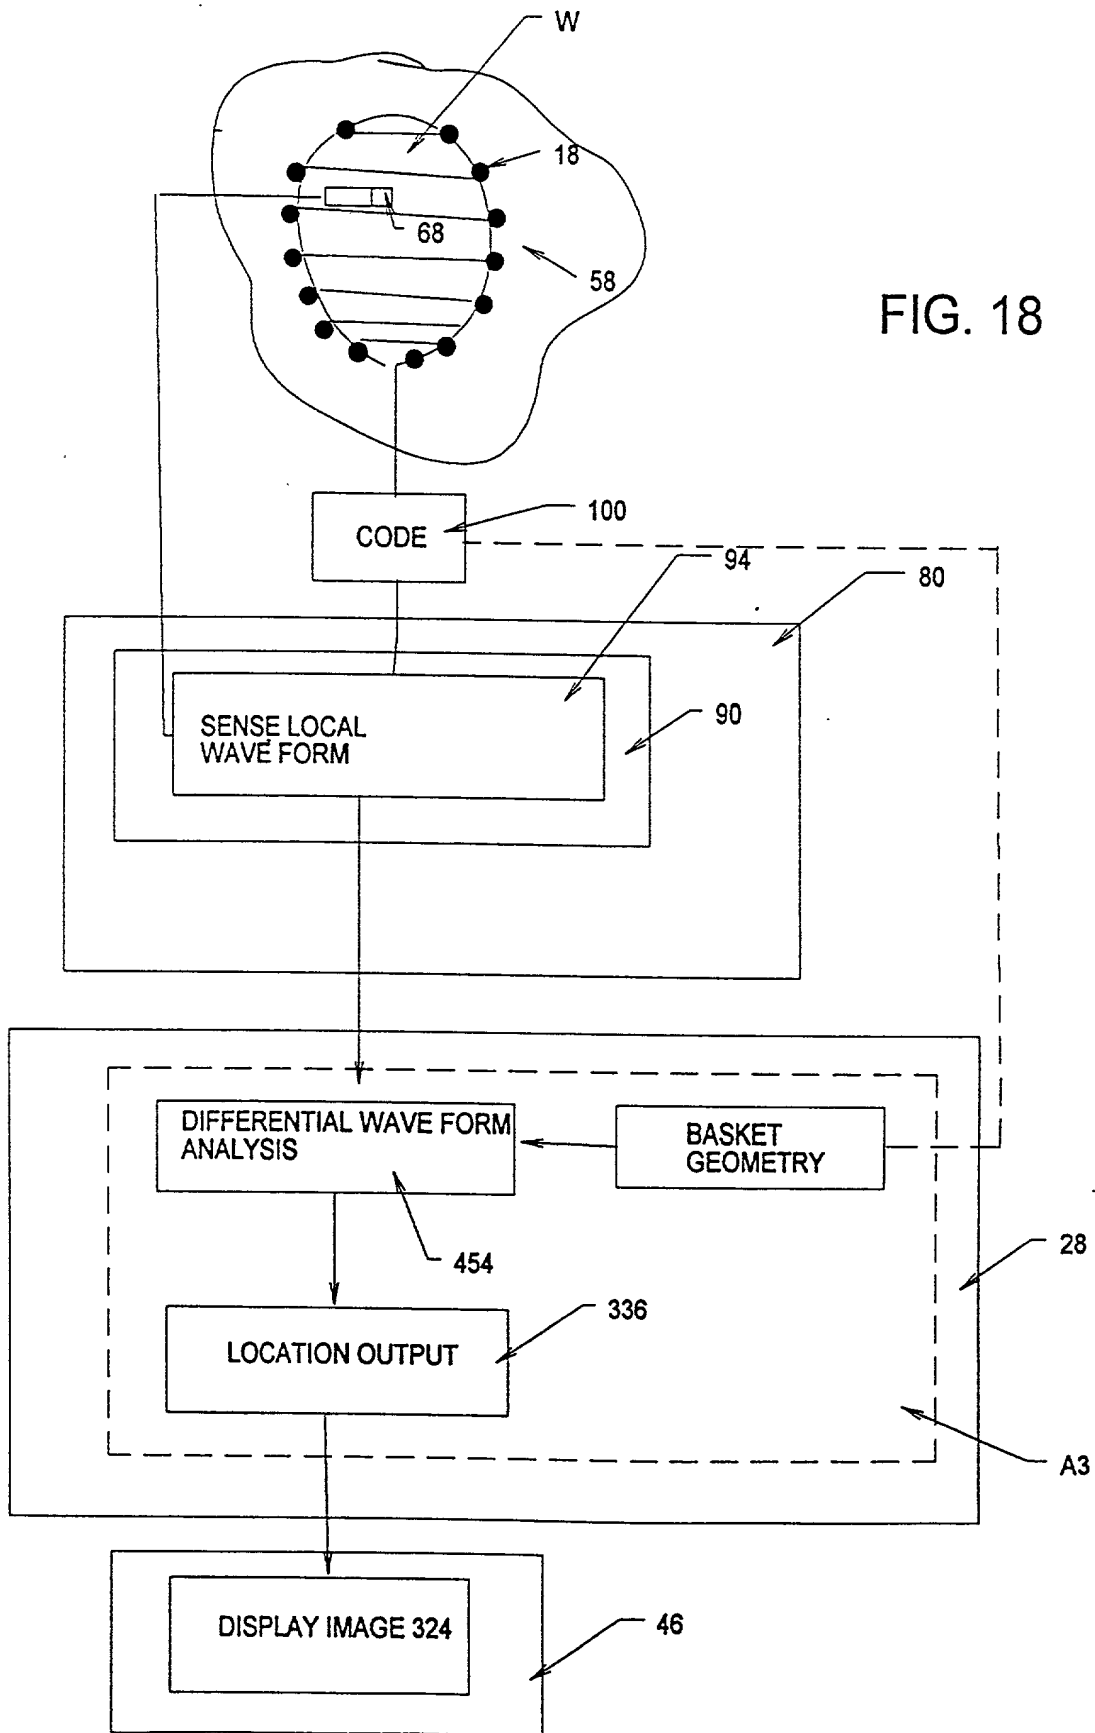


FIG. 19

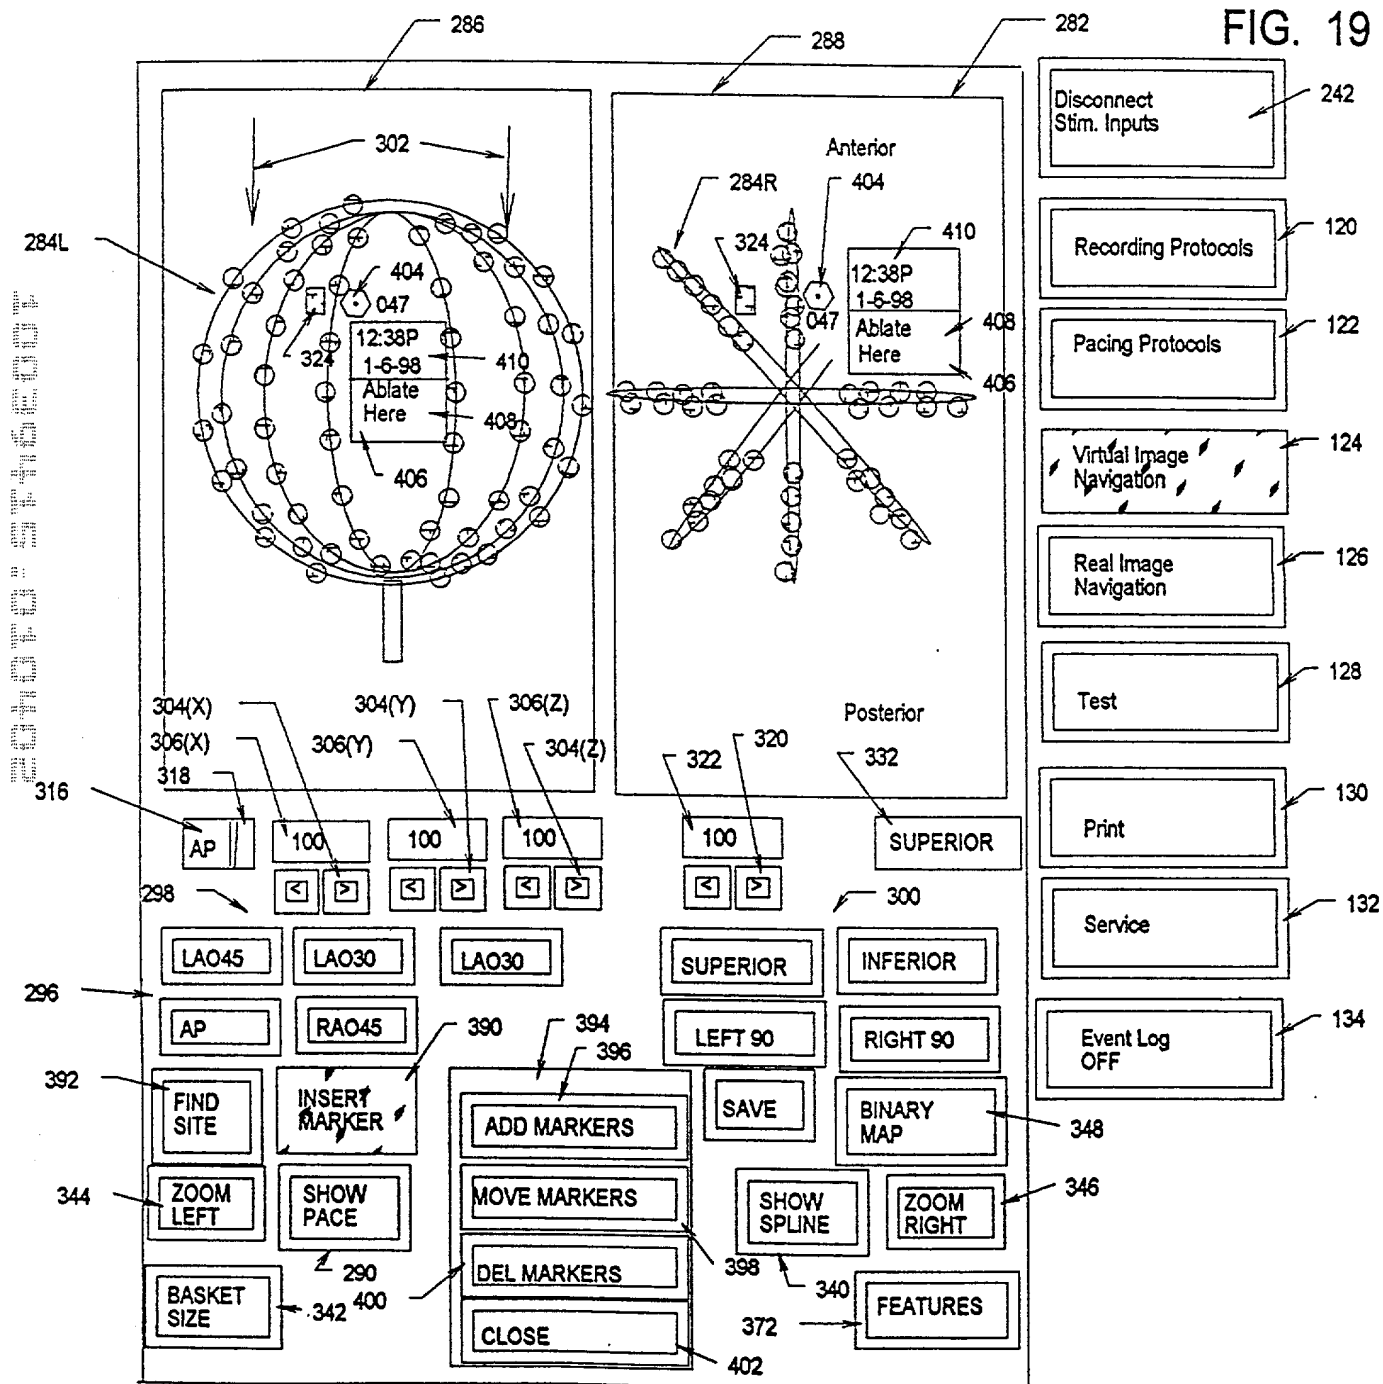


FIG. 20

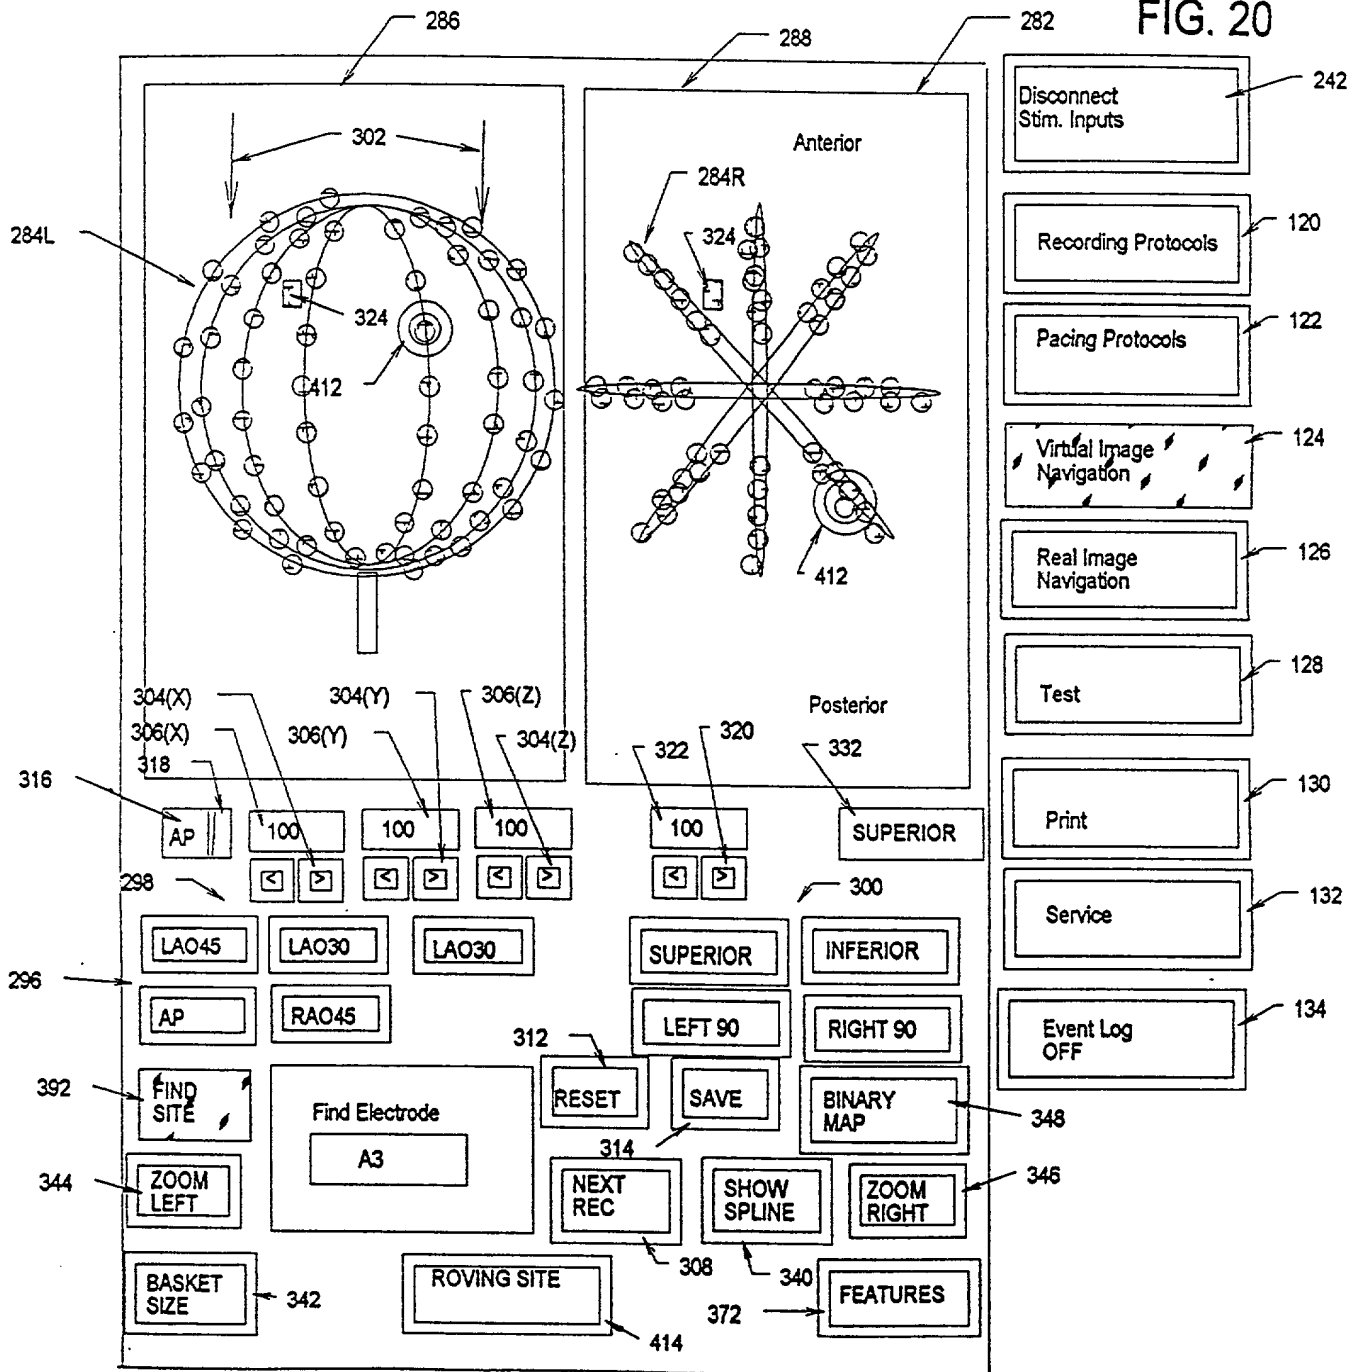


FIG. 21

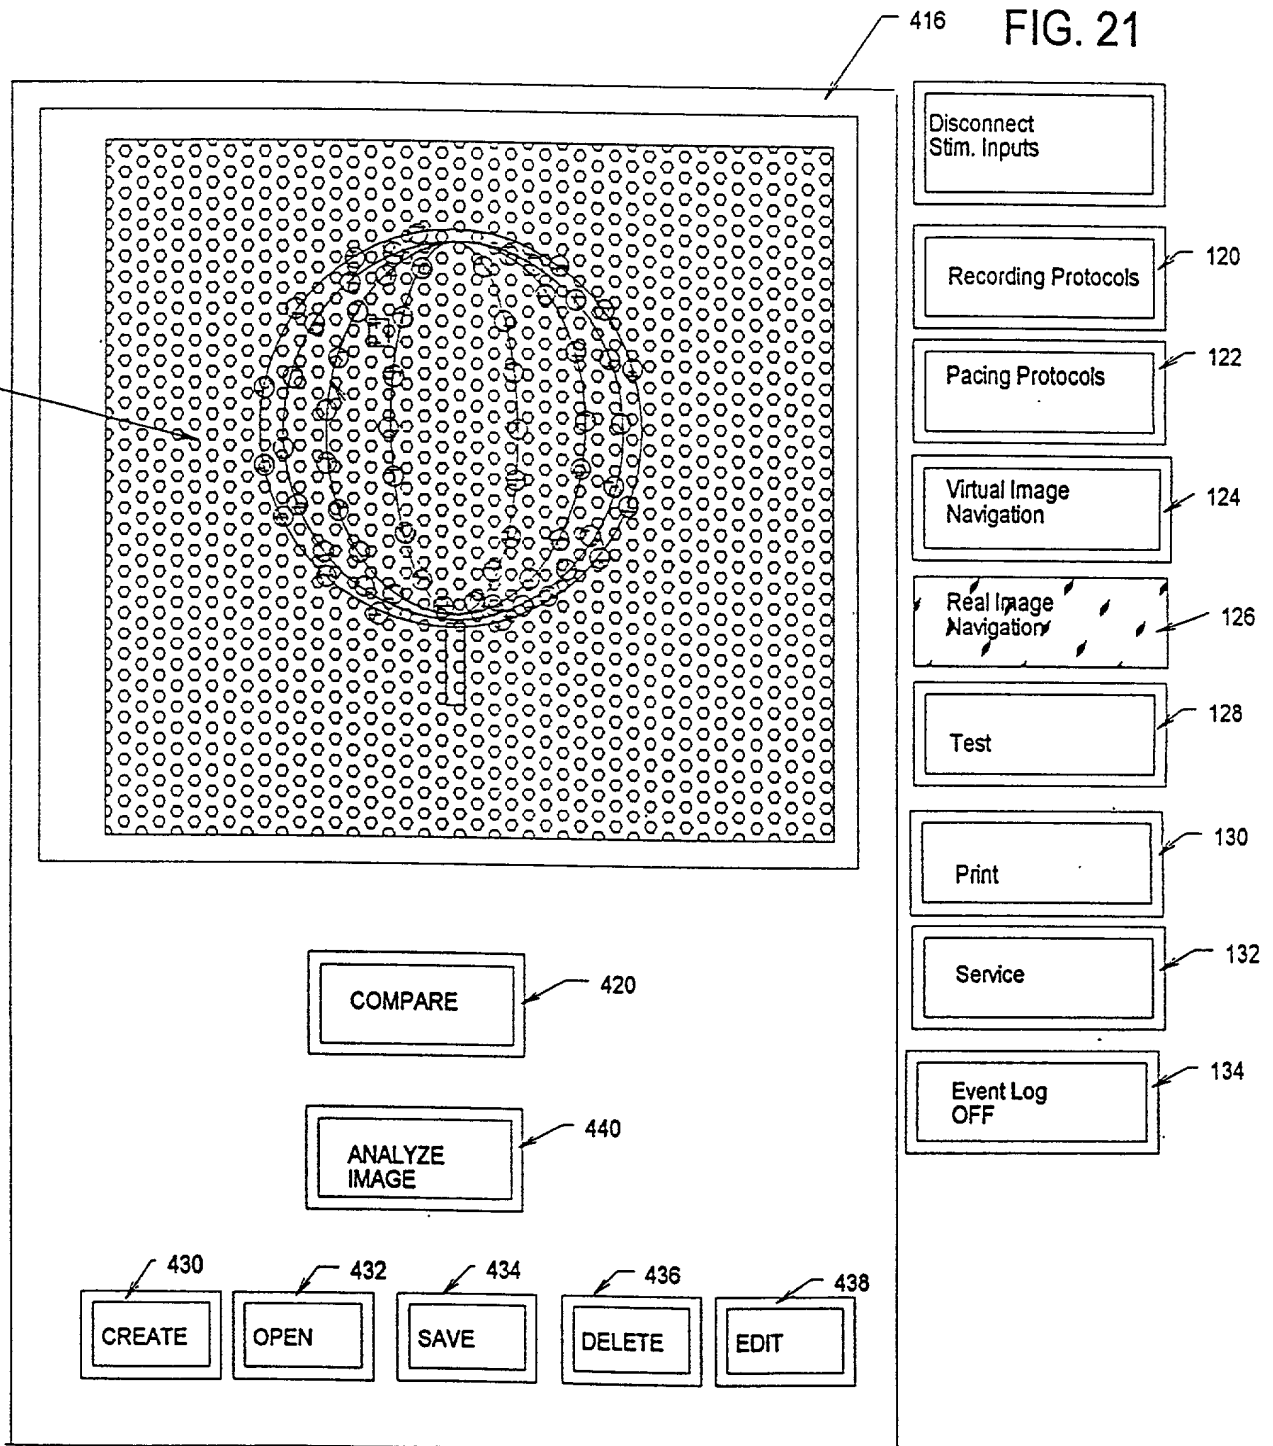
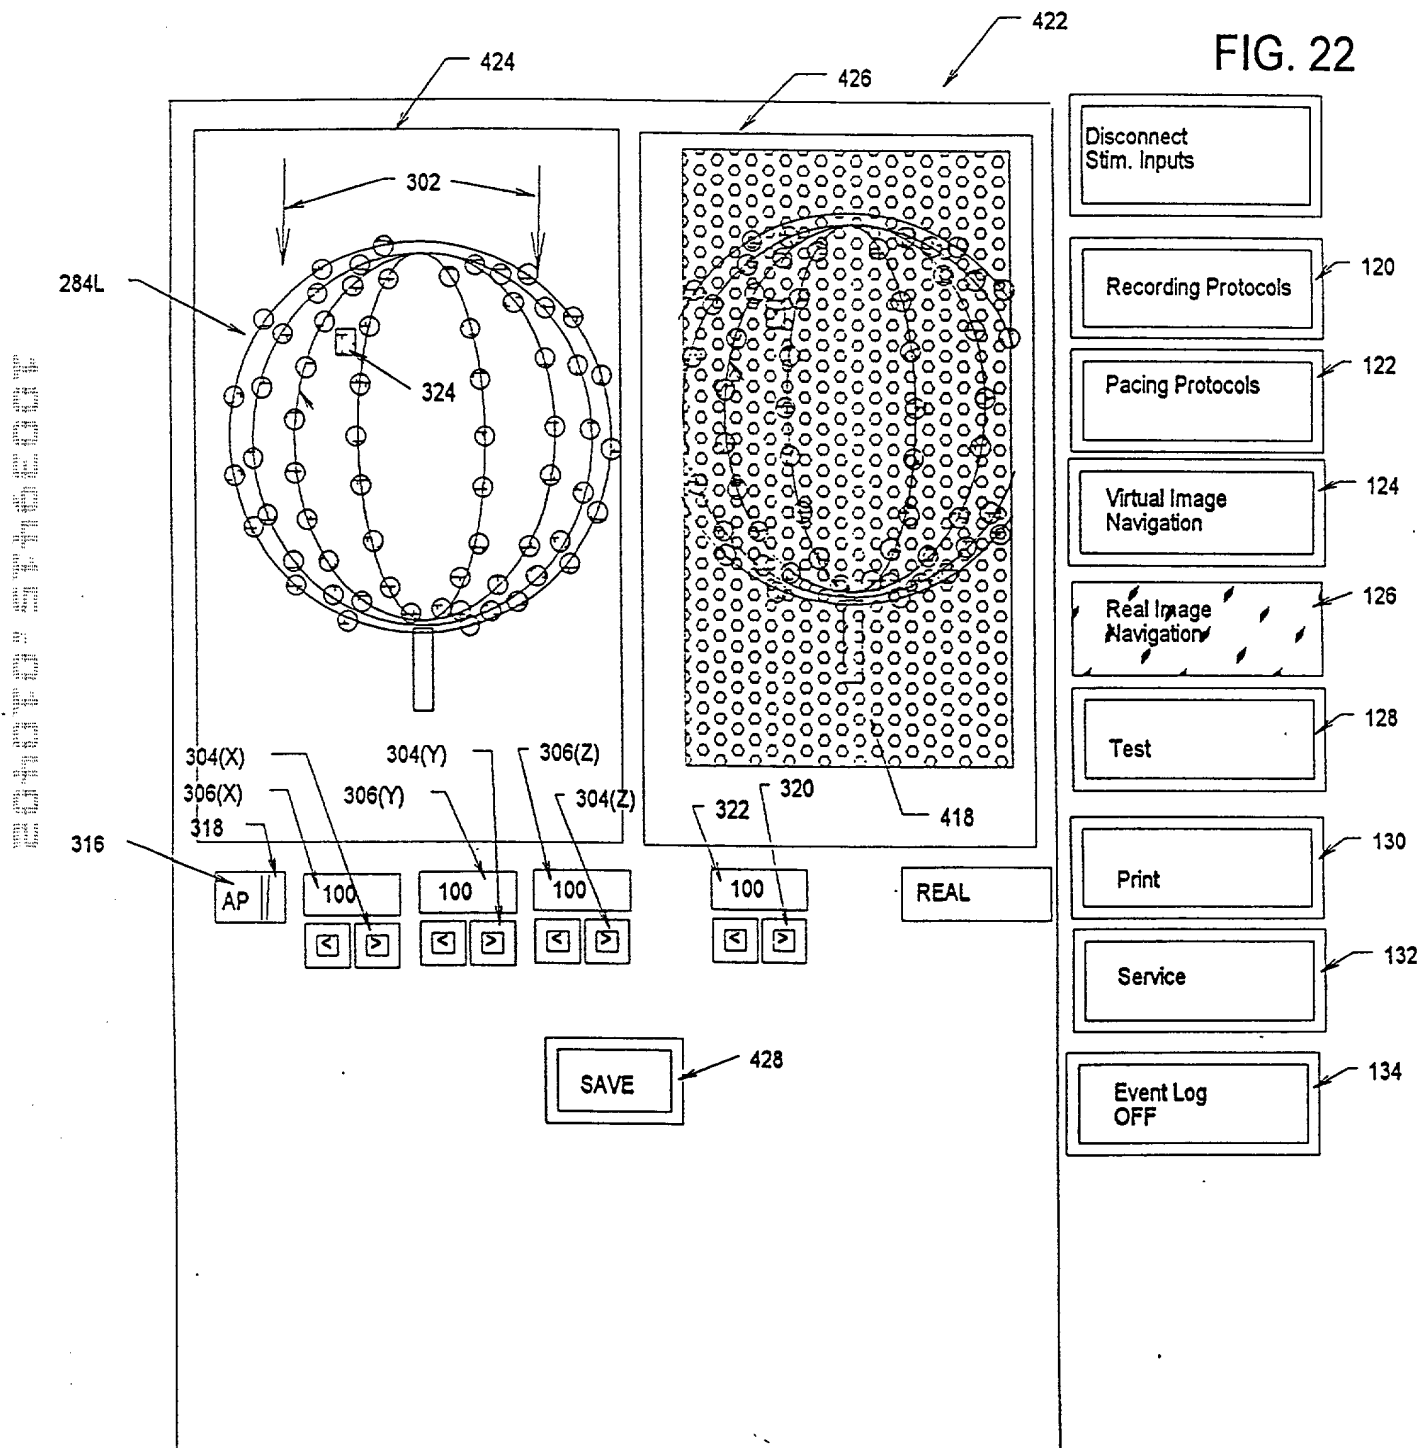


FIG. 22



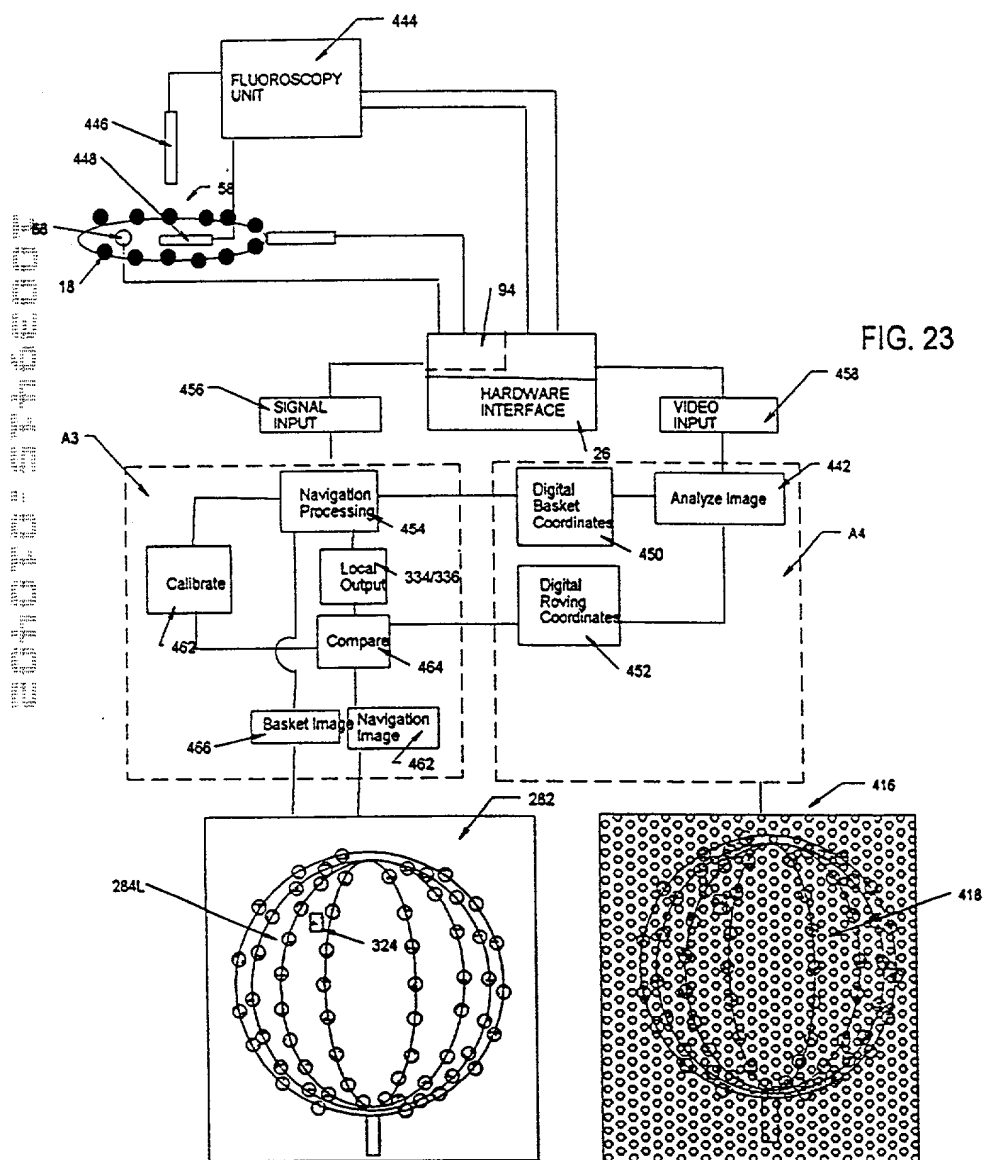


FIG. 24

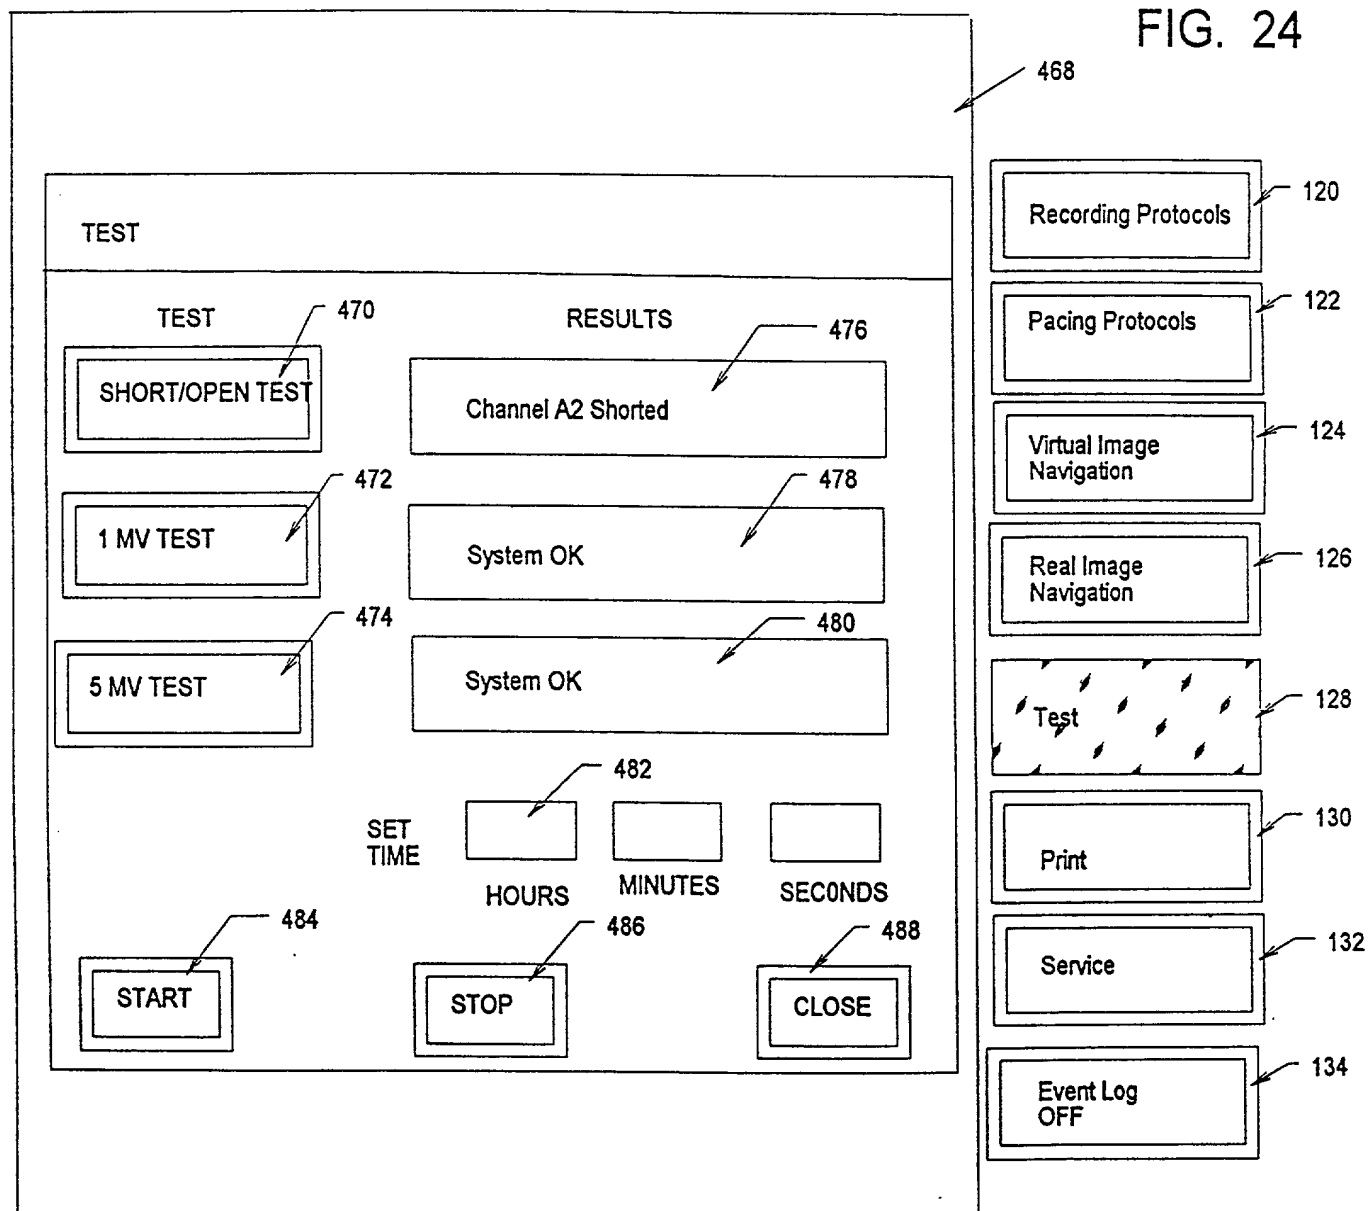


FIG. 25

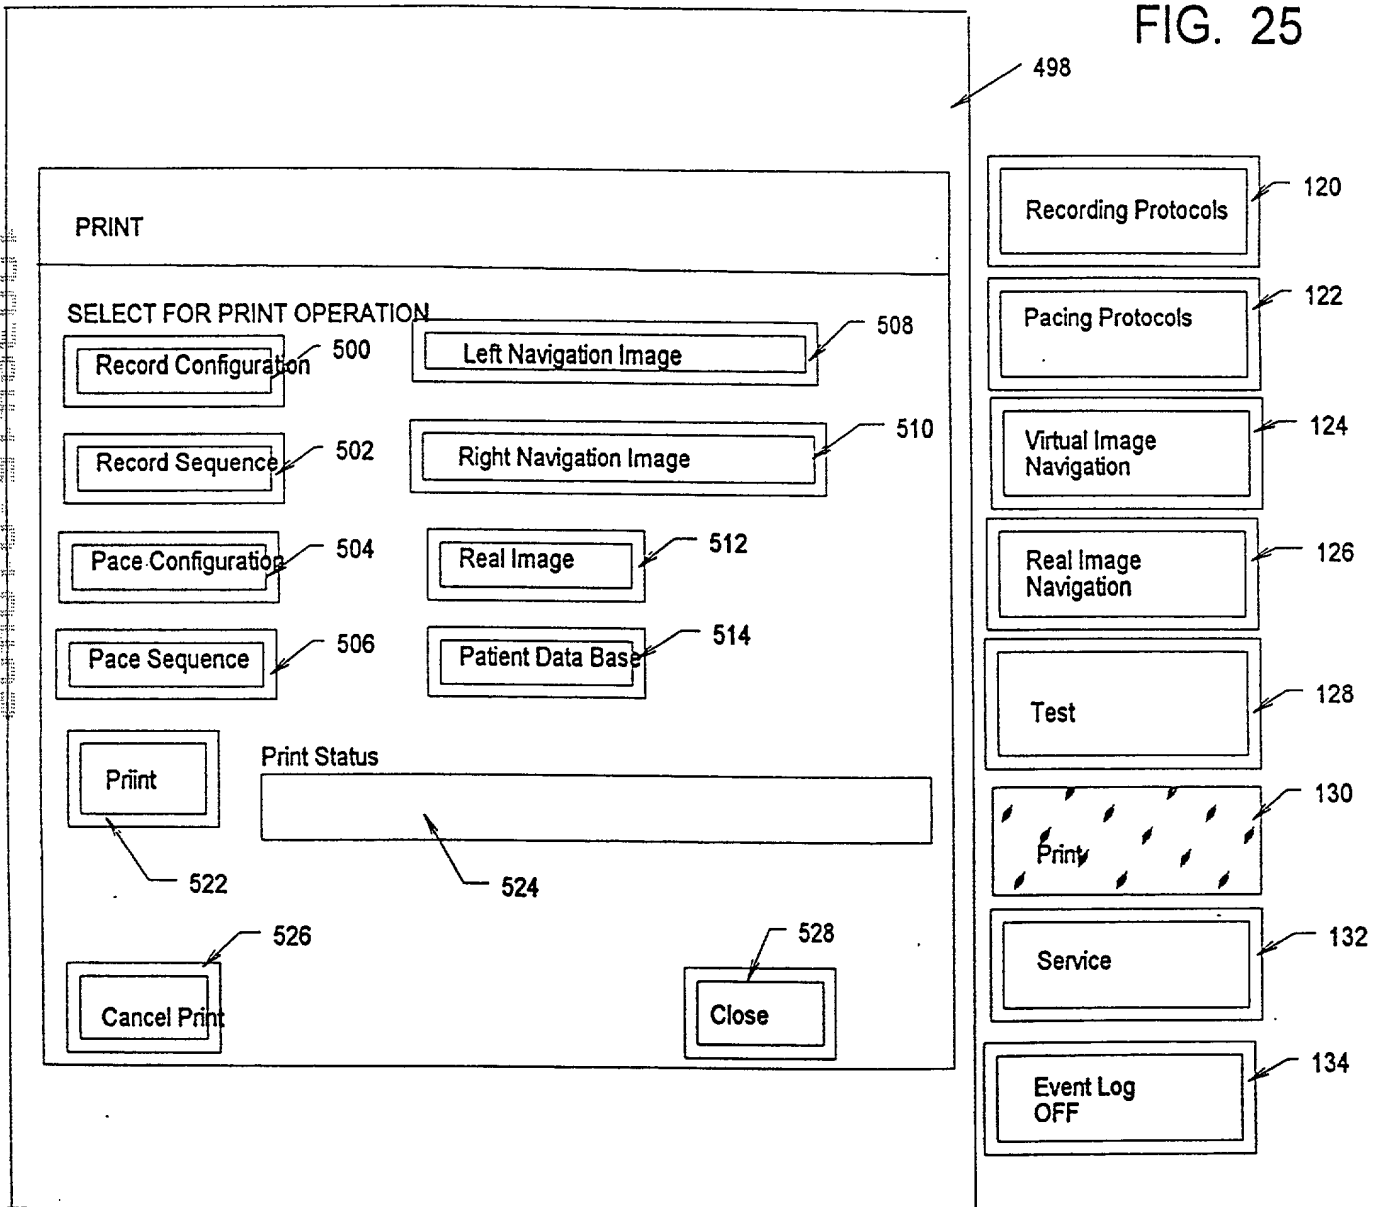


FIG. 26

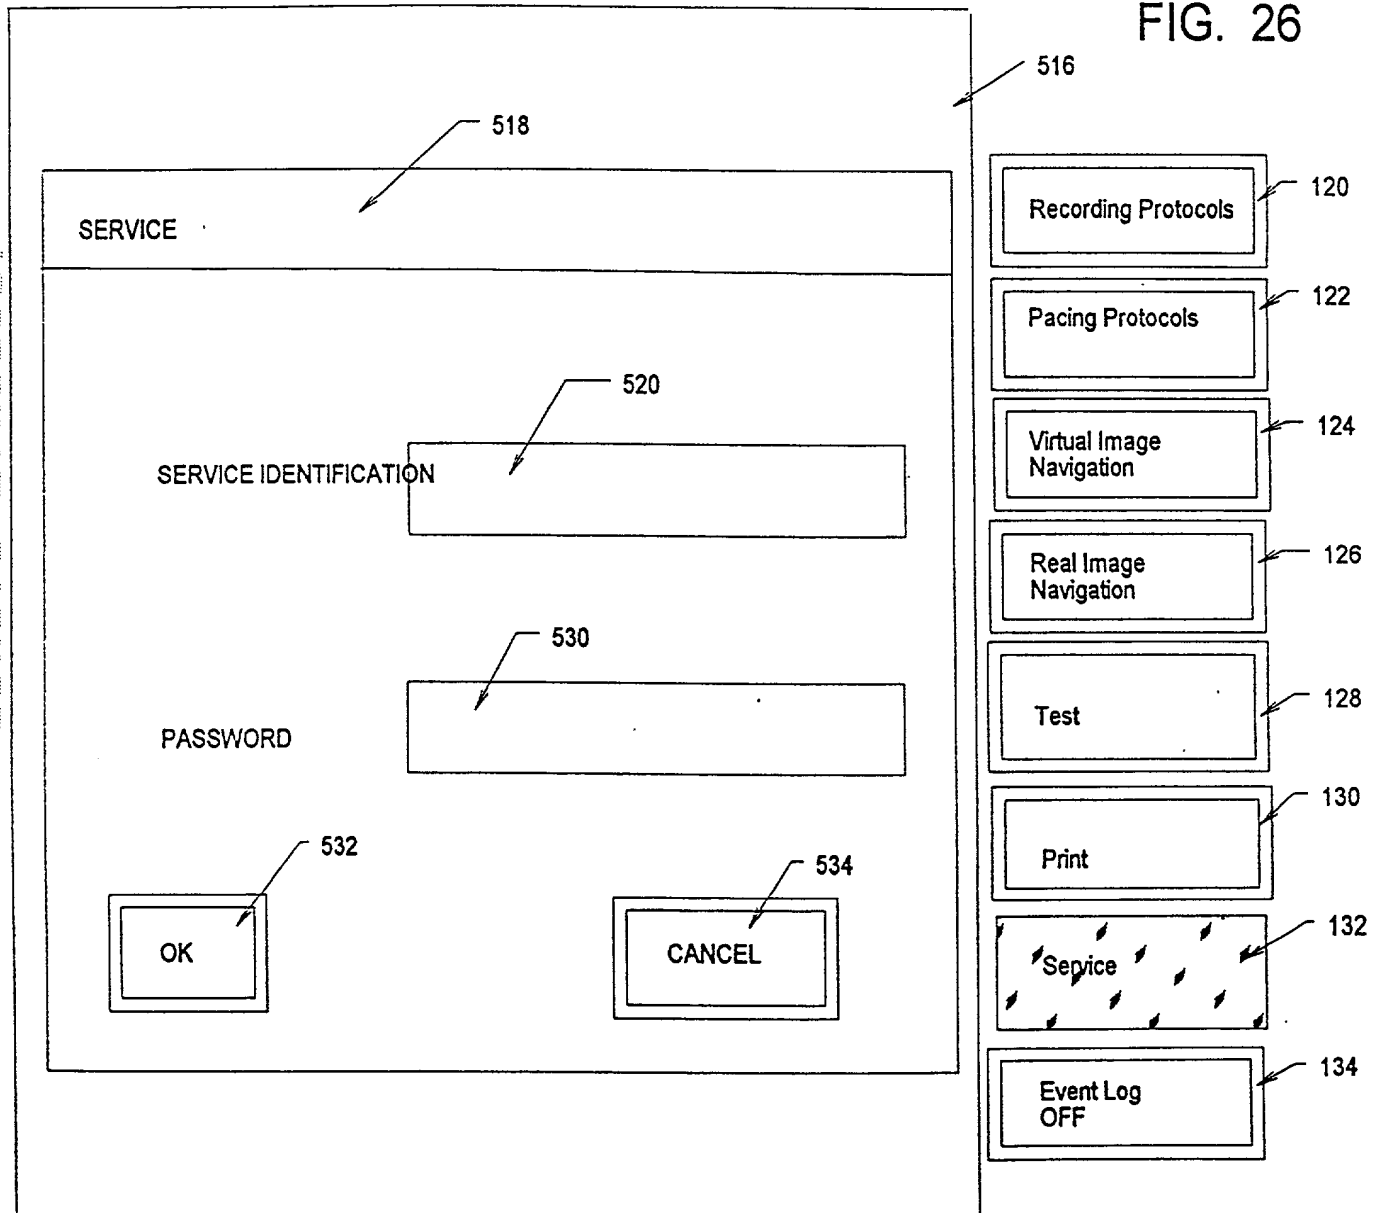


FIG. 27

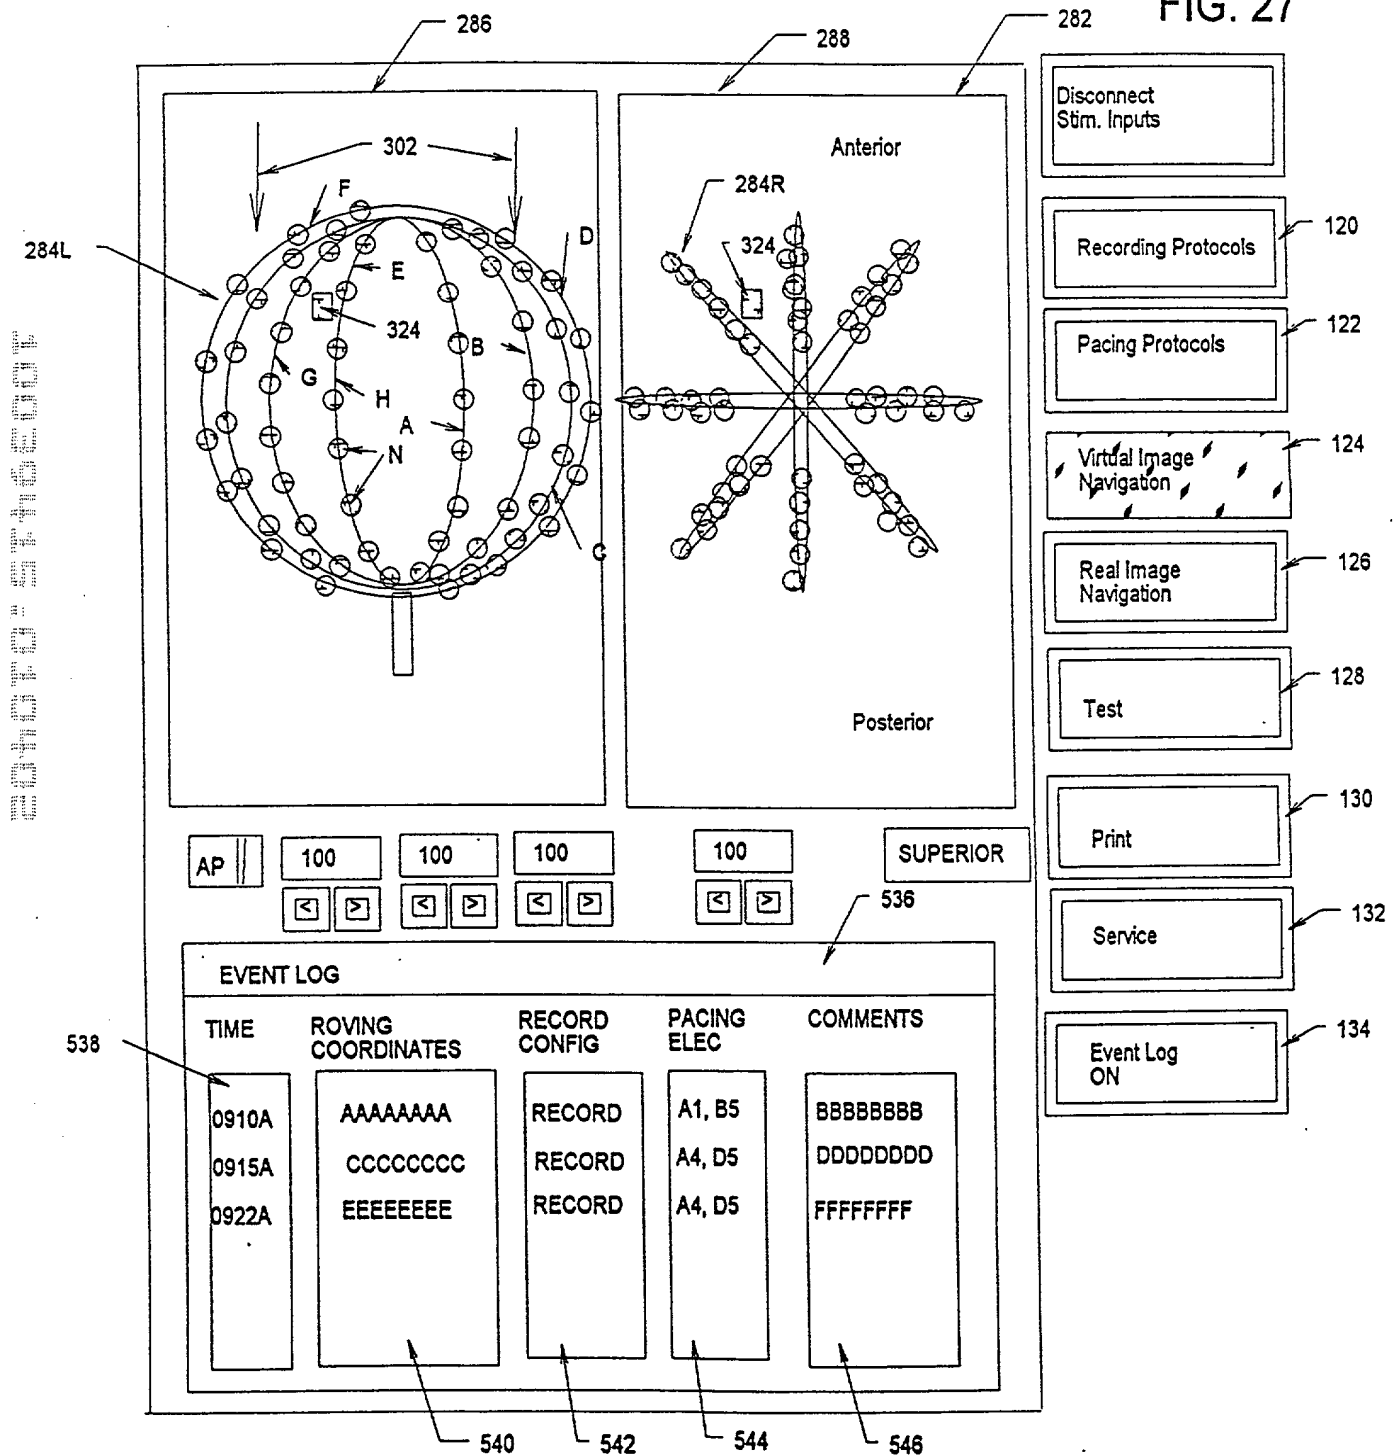


FIG. 28

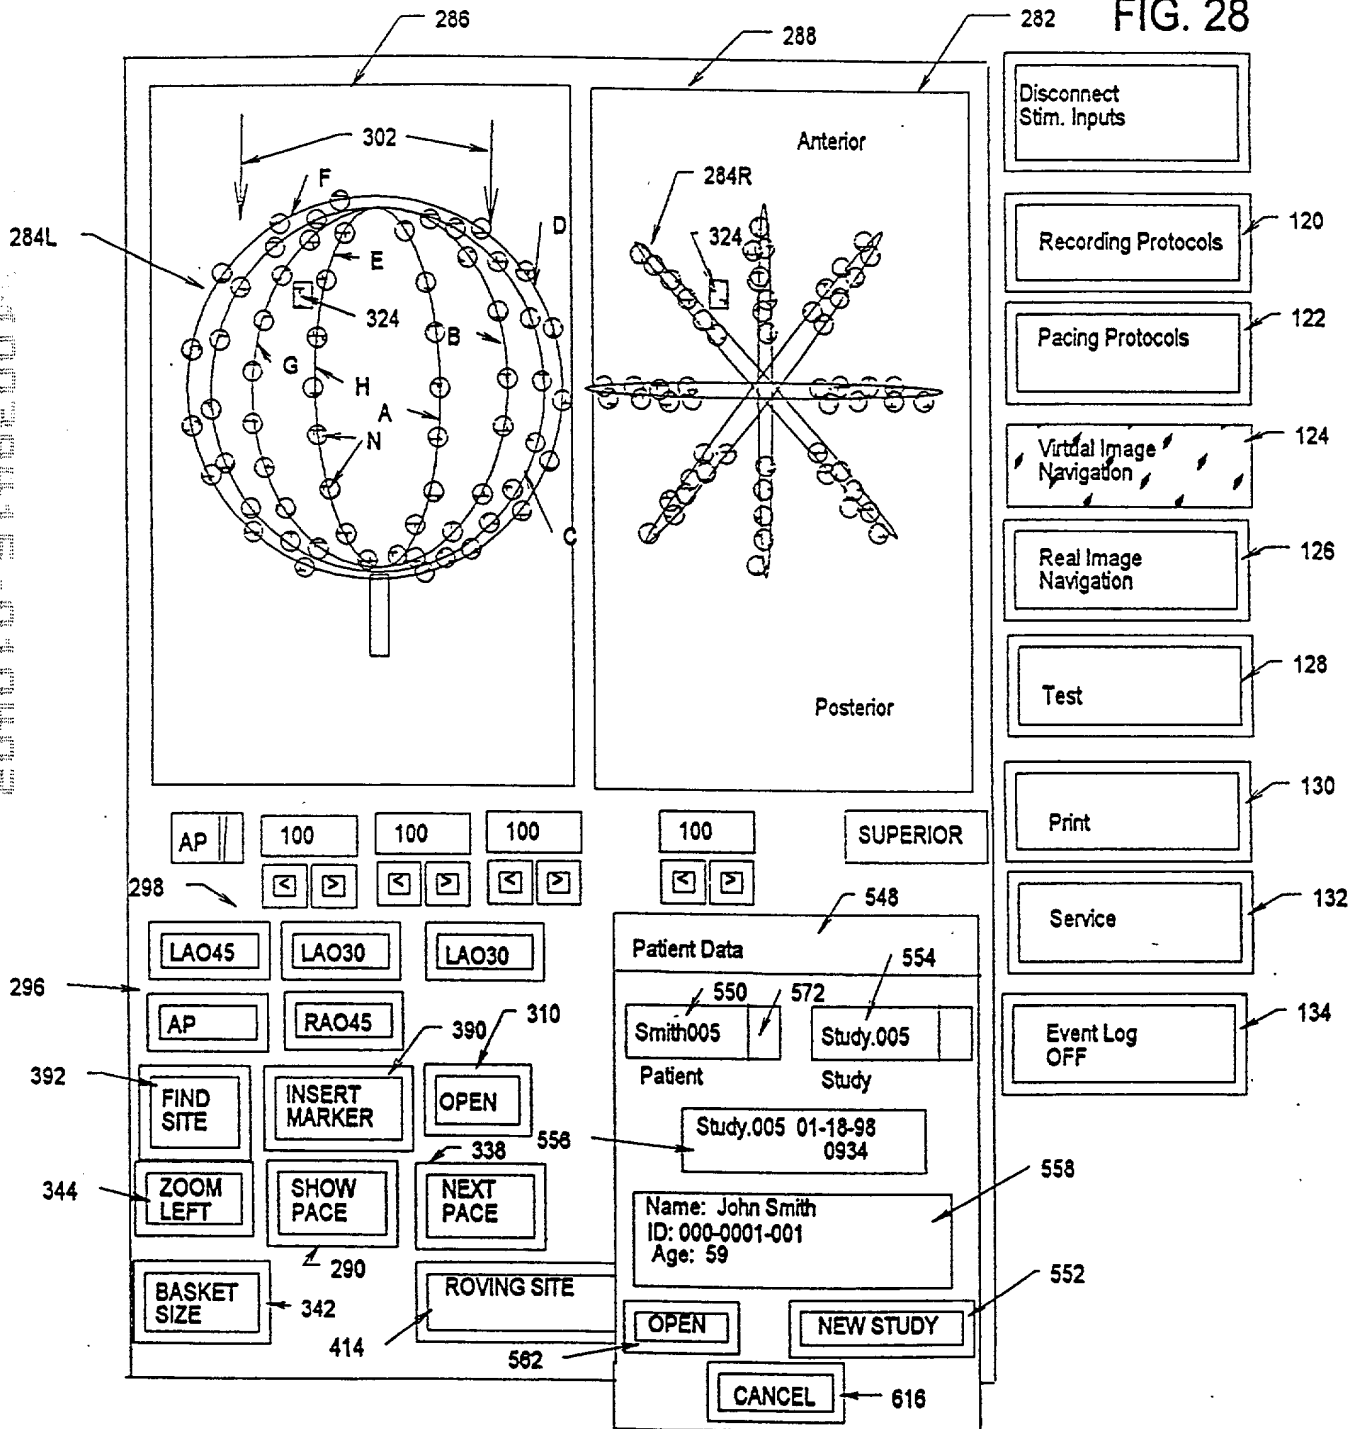


FIG. 29

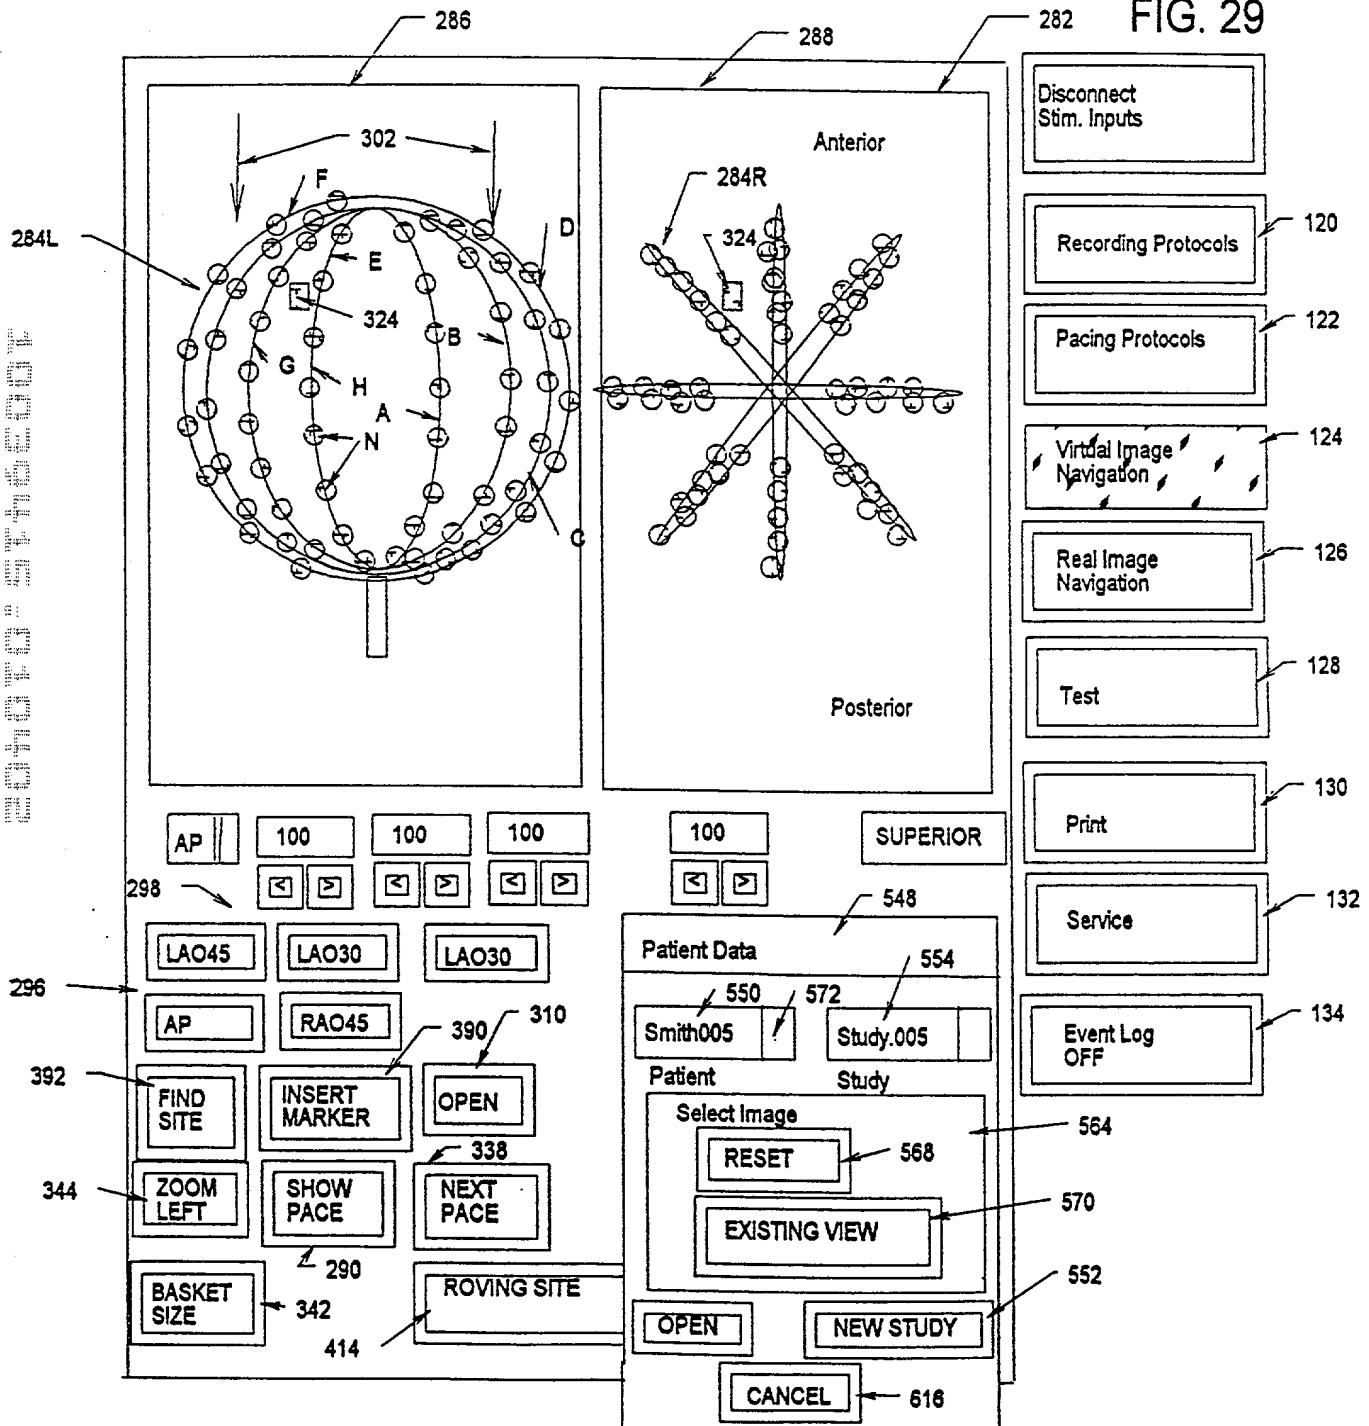


FIG. 30

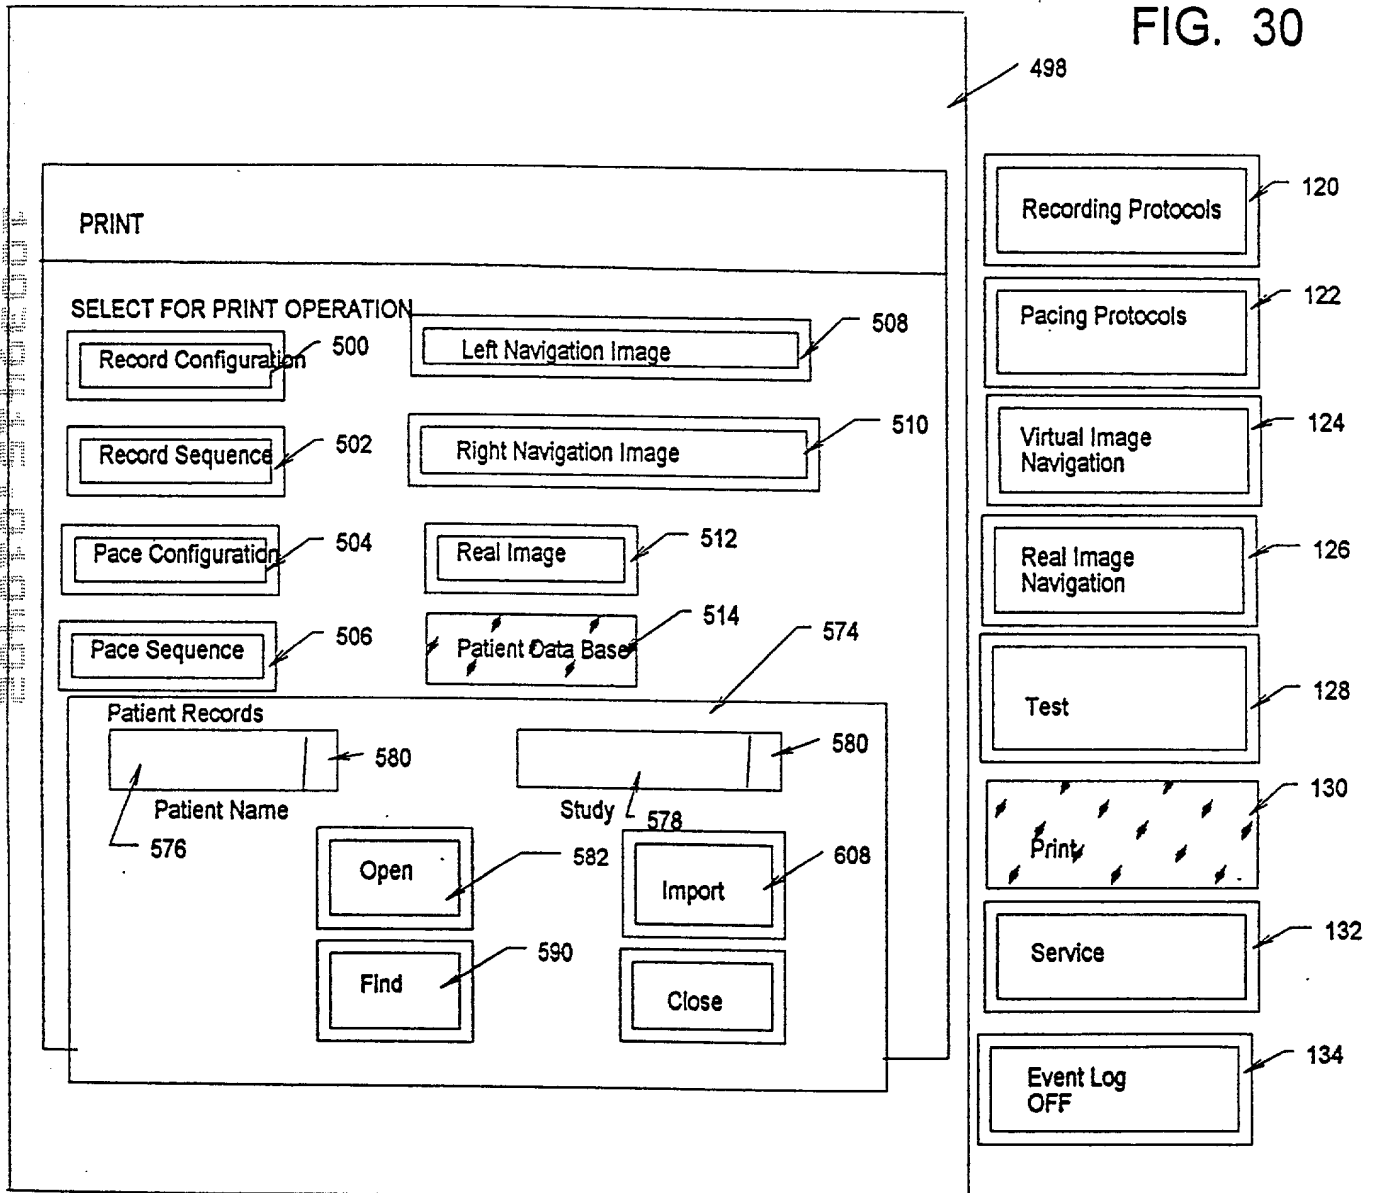


FIG. 31

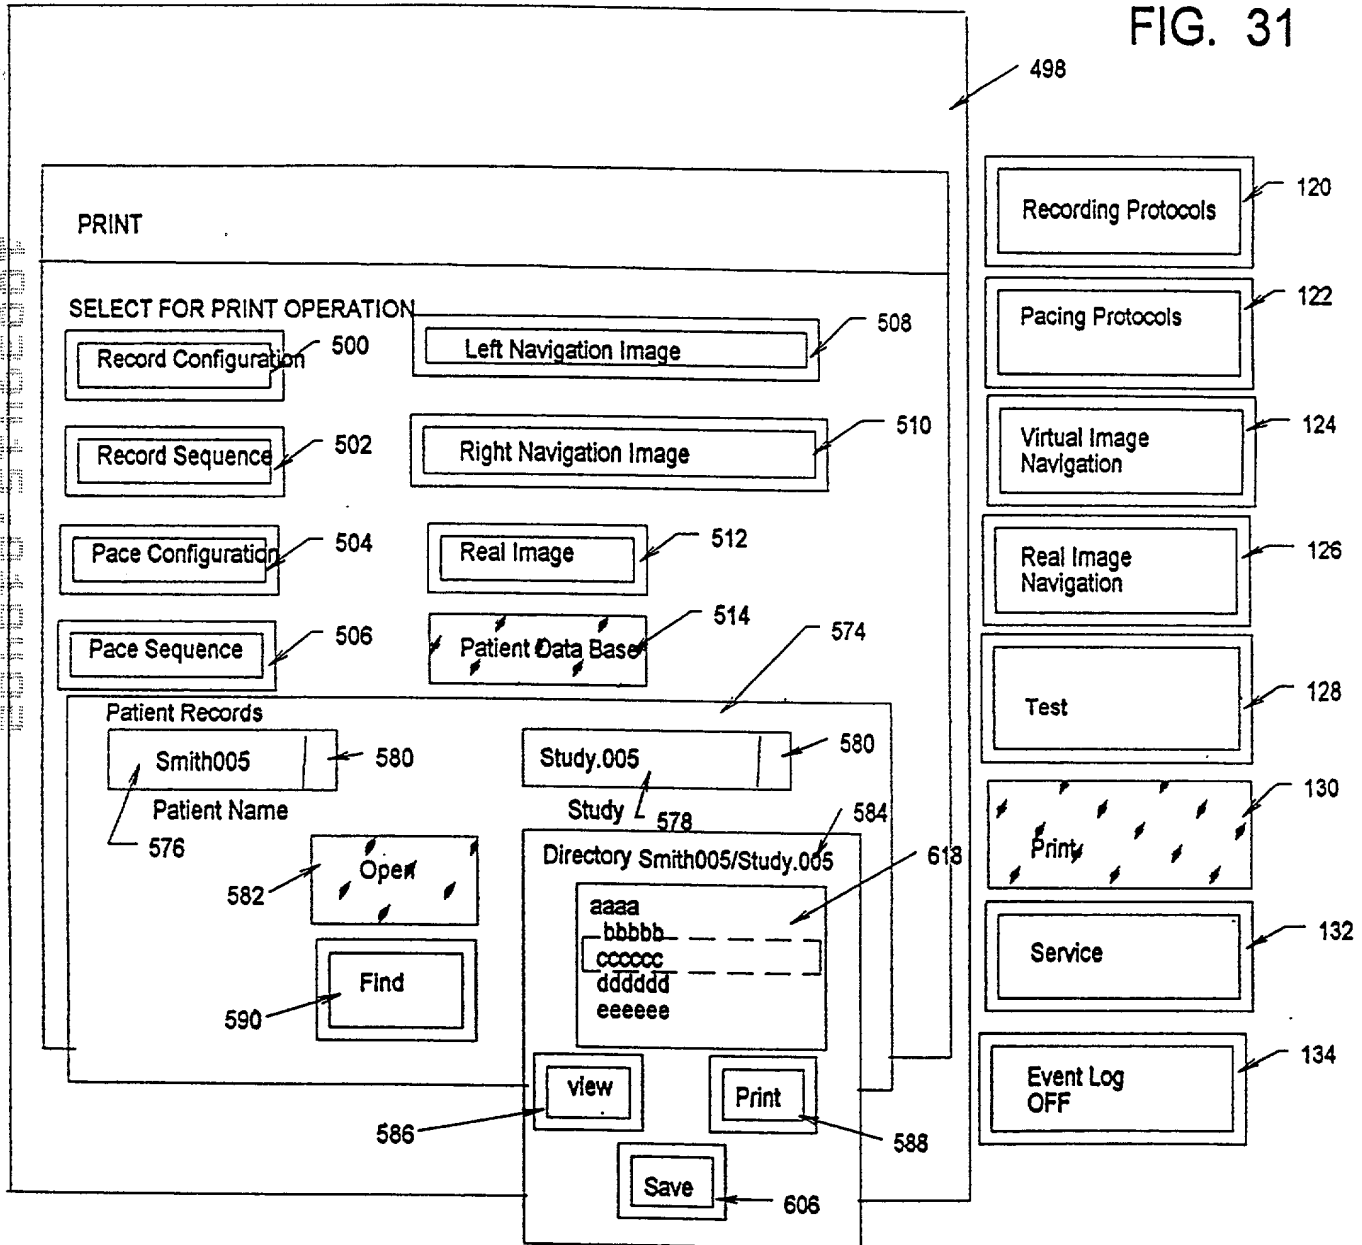


FIG. 32

